


**CAEN** n  
*Tools for Discovery*

# Register your device

Register your device to your **MyCAEN+** account and get access to our customer services, such as notification for new firmware or software upgrade, tracking service procedures or open a ticket for assistance. **MyCAEN+** accounts have a dedicated support service for their registered products. A set of basic information can be shared with the operator, speeding up the troubleshooting process and improving the efficiency of the support interactions.

**MyCAEN+** dashboard is designed to offer you a direct access to all our after sales services. Registration is totally free, to create an account go to <https://www.caen.it/become-mycaenplus-user> and fill the registration form with your data.

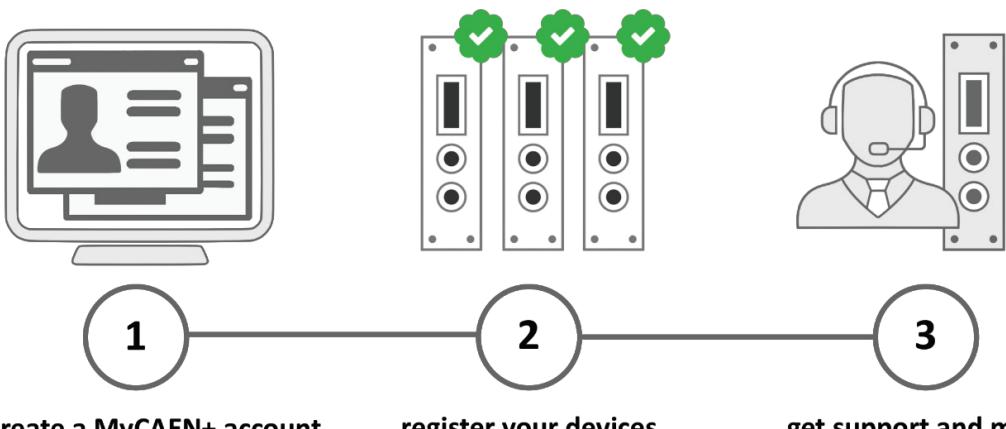

<https://www.caen.it/become-mycaenplus-user/>

## Purpose of this Manual



This document contains the full hardware description of the DT5751 CAEN digitizer and their principle of operating as **Waveform Recording Digitizer** (basing on the hereafter called "**waveform recording firmware**").

The reference firmware revision is: **4.16\_0.7**.

**For any reference to registers in this user manual, please refer to document [RD1] on the digitizer web page.**

**For any reference to DPP firmware in this user manual, please refer to documents [RD2] and [RD3] present on the firmware web page.**

## Change Document Record

Date	Revision	Changes
-	00-11	Old manuals are available on request (see Chap. <b>14</b> )
Jun 12 <sup>th</sup> , 2017	12	Revised layout and improved text
Dec 19 <sup>th</sup> , 2023	13	Revised layout and improved text. Added up-to-date: controllers and adapters support, accessories. Updated Chap. <b>3, 5, 11 and 13</b> . Updated Sec. <b>8.1, 8.2, 9.7.5, 9.8, 9.9, 9.11, 9.12</b>

## Symbols, Abbreviated Terms and Notation

ADC	Analog-to-Digital Converter
AMC	ADC & Memory Controller
DAQ	Data Acquisition
DAC	Digital-to-Analog Converter
DC	Direct Current
LVDS	Low-Voltage Differential Signal
PLL	Phase-Locked Loop
ROC	ReadOut Controller
TTT	Trigger Time Tag
USB	Universal Serial Bus


## Reference Documents

- [RD1] UM6009 – 751 Registers Description
- [RD2] UM5960 – CoMPASS User Manual
- [RD3] UM2764 – DPP-ZLEplus User Manual
- [RD4] UM2088 – DPP-PSD User Manual
- [RD5] GD2512 – CAENUpgrader QuickStart Guide
- [RD6] Precautions for Handling, Storage and Installation
- [RD7] AD9510. Available at [http://www.analog.com/UploadedFiles/Data\\_Sheets/AD9510.pdf](http://www.analog.com/UploadedFiles/Data_Sheets/AD9510.pdf)
- [RD8] AN6308 – Downsampling measurements with CAEN Digitizer 720/724/740/751 families
- [RD9] UM1935 – CAENDigitizer User & Reference Manual

- [RD10] UM2091 – CAEN WaveDump User Manual
- [RD11] GD2817 – How to make coincidences with CAEN digitizers
- [RD12] AN2086 – Synchronization of a multi-board acquisition systems with CAEN digitizers
- [RD13] AN2472 – CONET1 to CONET2 migration
- [RD14] UM4413 – A2818 Technical Information Manual
- [RD15] UM3121 – A3818 Technical Information Manual
- [RD16] DS7799 A4818 Adapter Data Sheet
- [RD17] GD2783 – First Installation Guide to Desktop Digitizers & MCA
- [RD18] UM1934 – CAENComm User & Reference Manual
- [RD19] GD2512 – CAENUpgrader QuickStart Guide
- [RD20] x751 Family DPP-PSD Firmware Compatibility

All CAEN documents can be downloaded at:  
[www.caen.it/support-services/documentation-area](http://www.caen.it/support-services/documentation-area)

## Manufacturer Contacts



### CAEN S.p.A.

Via Vетраia, 11 55049 Viareggio (LU) - ITALY  
Tel. +39.0584.388.398 Fax +39.0584.388.959  
[www.caen.it](http://www.caen.it) | [info@caen.it](mailto:info@caen.it)  
©CAEN SpA – 2017

## Limitation of Responsibility

If the warnings contained in this manual are not followed, CAEN will not be responsible for damage caused by improper use of the device. The manufacturer declines all responsibility for damage resulting from failure to comply with the instructions for use of the product. The equipment must be used as described in the user manual, with particular regard to the intended use, using only accessories as specified by the manufacturer. No modification or repair can be performed.

## Disclaimer

No part of this manual may be reproduced in any form or by any means, electronic, mechanical, recording, or otherwise, without the prior written permission of CAEN SpA.

The information contained herein has been carefully checked and is believed to be accurate; however, no responsibility is assumed for inaccuracies. CAEN SpA reserves the right to modify its products specifications without giving any notice; for up to date information please visit [www.caen.it](http://www.caen.it).

## Made in Italy

We remark that all our boards have been designed and assembled in Italy. In a challenging environment where a competitive edge is often obtained at the cost of lower wages and declining working conditions, we proudly acknowledge that all those who participated in the production and distribution process of our devices were reasonably paid and worked in a safe environment (while this is true for the boards marked "MADE IN ITALY", we cannot guarantee for third-party manufacturers).



# Index

<b>Purpose of this Manual</b> . . . . .	1
<b>Change document record</b> . . . . .	1
<b>Symbols, abbreviated terms and notation</b> . . . . .	1
<b>Reference Documents</b> . . . . .	1
<b>Manufacturer Contacts</b> . . . . .	3
<b>Limitation of Responsibility</b> . . . . .	3
<b>Disclaimer</b> . . . . .	3
<b>Made in Italy</b> . . . . .	3
<b>Safety Notices</b> . . . . .	7
<b>1 Introduction</b> . . . . .	9
<b>2 Block Diagram</b> . . . . .	11
<b>3 Technical Specifications</b> . . . . .	12
<b>4 Packaging and Compliancy</b> . . . . .	14
<b>5 PID (Product Identifier)</b> . . . . .	16
<b>6 Power Requirements</b> . . . . .	17
<b>7 Cooling Management</b> . . . . .	18
7.1 ADC chips temperature readout . . . . .	18
7.2 ADC chips over temperature protection . . . . .	18
7.3 Cleaning Air Vents . . . . .	18
<b>8 Panels Description</b> . . . . .	20
8.1 Front Panel . . . . .	21
8.2 Rear Panel . . . . .	23
<b>9 Functional Description</b> . . . . .	24
9.1 Analog Input Stage . . . . .	24
9.1.1 DC Offset Individual Setting . . . . .	24
9.2 Clock Distribution . . . . .	25
9.3 PLL Mode . . . . .	26
9.4 Reducing the Sampling Frequency . . . . .	26
9.5 Trigger Clock . . . . .	26
9.6 DES Mode . . . . .	26
9.7 Acquisition Modes . . . . .	27
9.7.1 Channel Calibration . . . . .	27
9.7.2 Acquisition Run/Stop . . . . .	30
9.7.3 Acquisition Triggering: Samples and Events . . . . .	30
9.7.4 Multi-Event Memory Organization . . . . .	32
9.7.4.1 Custom size events . . . . .	32
9.7.5 Event structure . . . . .	33
9.7.5.1 Header . . . . .	33

9.7.5.2	Data	35
9.7.5.3	Event Format Examples	35
9.7.6	Acquisition Synchronization	35
<b>9.8</b>	<b>Trigger Management</b>	<b>37</b>
9.8.1	Software Trigger	37
9.8.2	External Trigger	37
9.8.3	Self-Trigger	38
9.8.4	Trigger Coincidence Level	39
9.8.5	TRG-IN as Gate	41
9.8.6	Trigger distribution	41
9.8.6.1	Example	42
9.9	Multi-board Synchronization	43
9.10	Test Pattern Generator	44
9.11	Reset, Clear and Default Configuration	45
9.11.1	Global Reset	45
9.11.2	Memory Reset	45
9.11.3	Timer Reset	45
9.12	Data Transfer Capabilities and Events Readout	46
9.12.1	Block Transfer	46
9.12.2	Single Data Transfer	46
9.13	Optical Link and USB Access	47
<b>10</b>	<b>Drivers &amp; Libraries</b>	<b>48</b>
10.1	Drivers	48
10.2	Libraries	48
<b>11</b>	<b>Software Tools</b>	<b>50</b>
11.1	CAENUpgrader	50
11.2	CAENComm Demo	51
11.3	CAEN WaveDump	52
11.4	CoMPASS	53
11.5	DPP-ZLEplus Control Software	54
<b>12</b>	<b>HW Installation</b>	<b>55</b>
12.1	Power-on Status	56
<b>13</b>	<b>Firmware and Upgrades</b>	<b>57</b>
13.1	Firmware Upgrade	57
13.1.1	Firmware File Description	58
13.2	Troubleshooting	58
<b>14</b>	<b>Technical Support</b>	<b>59</b>

## List of Figures

<b>Fig. 2.1</b>	Block Diagram.	11
<b>Fig. 5.1</b>	PID location on DT5751 (the number in the picture is purely indicative).	16
<b>Fig. 6.1</b>	AC/DC power supply provided with the module.	17
<b>Fig. 8.1</b>	Front panel view.	20

<b>Fig. 8.2</b>	Rear panel view. . . . .	20
<b>Fig. 9.1</b>	Analog input diagram. . . . .	24
<b>Fig. 9.2</b>	Clock distribution diagram. . . . .	25
<b>Fig. 9.3</b>	Diagram of the ADCcalibration flow. . . . .	27
<b>Fig. 9.4</b>	Automatic calibration at WaveDump first run. . . . .	28
<b>Fig. 9.5</b>	Temperature monitoring with manual calibration in WaveDump software. . . . .	29
<b>Fig. 9.6</b>	Channel calibration in CoMPASS Software. . . . .	29
<b>Fig. 9.7</b>	Trigger Overlap. . . . .	31
<b>Fig. 9.8</b>	TTT description. . . . .	34
<b>Fig. 9.9</b>	ETTT description. . . . .	34
<b>Fig. 9.10</b>	Event Format in Normal Mode. . . . .	35
<b>Fig. 9.11</b>	Block diagram of Trigger management. . . . .	37
<b>Fig. 9.12</b>	Self-trigger generation. . . . .	38
<b>Fig. 9.13</b>	Self-trigger relationship with Majority level = 0. . . . .	39
<b>Fig. 9.14</b>	Self-trigger relationship with Majority level = 1 and $T_{TVAW} \neq 0$ . . . . .	40
<b>Fig. 9.15</b>	Self-trigger relationship with Majority level = 1 and $T_{TVAW} = 0$ . . . . .	41
<b>Fig. 9.16</b>	Trigger configuration of TRG-OUT front panel connector. . . . .	42
<b>Fig. 9.17</b>	FPGA Test Waveform. . . . .	44
<b>Fig. 10.1</b>	Drivers and software layers. . . . .	49
<b>Fig. 11.1</b>	CAENUpgrader Graphical User Interface. . . . .	50
<b>Fig. 11.2</b>	CAENComm Demo Java and LabVIEW graphical interface. . . . .	51
<b>Fig. 11.3</b>	CAEN WaveDump. . . . .	52
<b>Fig. 11.4</b>	CoMPASS software tool. . . . .	53
<b>Fig. 11.5</b>	Screen-shots of DPP-ZLEplus Control Software. . . . .	54
<b>Fig. 12.1</b>	Front panel LEDs status at power-on. . . . .	56

## List of Tables

<b>Tab. 1.1</b>	Table of models and related items. . . . .	10
<b>Tab. 3.1</b>	Specification table. . . . .	13
<b>Tab. 4.1</b>	Delivered kit content. . . . .	14
<b>Tab. 9.1</b>	Buffer organization of 751 family series. For each value of buffer size it is reported the memory size and the number of samples of one buffer, where $k = 1024$ and $M = 1024 \cdot 1024$ . . . . .	32
<b>Tab. 9.2</b>	Reserved/Trg Options configuration table. . . . .	33

# Safety Notices

**N.B. Read carefully the “Precautions for Handling, Storage and Installation document provided with the product before starting any operation.**

The following HAZARD SYMBOLS may be reported on the unit:

	Caution, refer to product manual
	Caution, risk of electrical shock
	Protective conductor terminal
	Earth (Ground) Terminal
	Alternating Current
	Three-Phase Alternating Current

The following symbol may be reported in the present manual:

	General warning statement
---	---------------------------

The symbol could be accompanied by the following terms:

- **DANGER:** indicates a hazardous situation which, if not avoided, will result in serious injury or death.
- **WARNING:** indicates a hazardous situation which, if not avoided, could result in death or serious injury.
- **CAUTION:** indicates a situation or condition which, if not avoided, could cause physical injury or damage the product and / or the surrounding environment.

**CAUTION:** To avoid potential hazards



**USE THE PRODUCT ONLY AS SPECIFIED.  
ONLY QUALIFIED PERSONNEL SHOULD PERFORM SERVICE  
PROCEDURES**

**CAUTION:** Avoid Electric Overload



**TO AVOID ELECTRIC SHOCK OR FIRE HAZARD, DO NOT POWER A LOAD OUTSIDE OF ITS SPECIFIED RANGE**

**CAUTION:** Avoid Electric Shock



**TO AVOID INJURY OR LOSS OF LIFE, DO NOT CONNECT OR DISCONNECT CABLES WHILE THEY ARE CONNECTED TO A VOLTAGE SOURCE**

**CAUTION:** Do Not Operate without Covers



**TO AVOID ELECTRIC SHOCK OR FIRE HAZARD, DO NOT OPERATE THIS PRODUCT WITH COVERS OR PANELS REMOVED**

**CAUTION:** Do Not Operate in Wet/Damp Conditions



**TO AVOID ELECTRIC SHOCK, DO NOT OPERATE THIS PRODUCT IN WET OR DAMP CONDITIONS**

**CAUTION:** Do Not Operate in an Explosive Atmosphere



**TO AVOID INJURY OR FIRE HAZARD, DO NOT OPERATE THIS PRODUCT IN AN EXPLOSIVE ATMOSPHERE**



**THIS DEVICE SHOULD BE INSTALLED AND USED BY SKILLED TECHNICIAN ONLY OR UNDER HIS SUPERVISION**



**DO NOT OPERATE WITH SUSPECTED FAILURES.  
IF YOU SUSPECT THIS PRODUCT TO BE DAMAGED, PLEASE CONTACT THE TECHNICAL SUPPORT**

See Chap. 14 for the Technical Support contacts.

# 1 Introduction

The Mod. DT5751 is 2/4 Channel 10 1 GS/s Desktop Waveform Digitizer with 1 V<sub>pp</sub> input dynamic range on single ended MCX coaxial connectors (see **Tab. 1.1**). Versions with 200 mV<sub>pp</sub> single ended customization is also available (see **Tab. 1.1**). The DC offset is adjustable via a 16-bit DAC on each channel in the  $\pm 0.5$  V (@1 V<sub>pp</sub>),  $\pm 100$  mV (@200 mV<sub>pp</sub>) range. The digitizer can work in Dual Edge Sampling (DES mode) at 2 GS/s. In this mode only half of the channels are enabled for acquisition.

Considering the sampling frequency and bit number, these 751 digitizer family is well suited for fast signals as the ones coming from fast organic, inorganic and liquid scintillators coupled with PMTs or Silicon Photomultiplier, Diamond detectors and others.

A common acquisition trigger signal (common to all the channels) can be fed externally via the front panel TRG-IN input connector or via software. Alternatively, each channel is able to generate a self-trigger when the input signal goes under/over a programmable threshold. The trigger from one board can be propagated out of the board through the front panel GPO connector.

During the acquisition, data stream is continuously written in a circular memory buffer. When the trigger occurs, the digitizer writes additional samples for the post trigger and freezes the buffer that can be read by one of the provided readout links.

Each channel has a SRAM digital memory (see **Tab. 1.1** for the available memory size options) divided into buffers of programmable size (1  $\div$  1024). The size of the memory doubles when working in DES mode. The readout (from USB or Optical link) of a frozen buffer is independent from the write operations in the active circular buffer (ADC data storage).

DT5751 features front panel CLK-IN connector as well as an internal PLL for clock synthesis (50 MHz oscillator) from internal/external references.

The board houses USB 2.0 and optical link interfaces. USB 2.0 allows data transfers up to 30 MB/s. The Optical Link interface (CAEN proprietary CONET protocol) is capable of transfer rate up to 80 MB/s and offers daisy chain capability. Therefore, it is possible to connect up to 8 ADC modules to a single A4818 Adapter (or to a single A2818 Optical Link Controller, Obsolete), or up to 32 using a 4-link A3818 version (see **Tab. 1.1**).

In addition to the waveform recording firmware, CAEN provides for this digitizer two types of Digital Pulse Processing firmware (DPP):

- Pulse Shape Discrimination (DPP-PSD) **[RD4]**, which combines the functionalities of a digital QDC (charge integration) and discriminator of different shapes for particle identification.
- Zero Length Encoding (DPP-ZLEplus) **[RD3]**, for the Zero suppression and data reduction.

These special firmware make the digitizer an enhanced system for Physics Applications.

Board Model	Description
DT5751	2/4 Ch. 10 bit 2/1 GS/s Digitizer: 3.6/1.8MS/ch, EP3C16, SE
WPERS0175102	x751 Customization - 200 mVpp Input Range, SE
DPP Firmware	Description
DDP-PSD	DDP-PSD Digital Pulse Processing for Pulse Shape Discrimination
DDP-ZLEplus	Digital Pulse Processing Zero Length Encoding
Related Products	Description
A3818A	A3818A – PCIe 1 Optical Link
A3818B	A3818B – PCIe 2 Optical Link
A3818C	A3818C – PCIe 4 Optical Link
A4818	A4818 - USB3 to Conet2 Adapter
A2818 (Obsolete)	A2818 – PCI Optical Link (Rhos compliant)

Accessories	Description
DT4700	Clock Generator and FAN-OUT
A317	Cable assembly for Clock distribution 3-pin AMPMODU IV female terminations - 18 cm
A317L	Cable assembly for Clock distribution 3-pin AMPMODU IV female terminations - 25 cm
A318	Adapter for Clock signal FISCHER S101A004 male to 3-pin AMPMODU IV female - 10 cm
A319B	A319B - Clock Cable for Digitizer Series 1.0 to 2.0 interconnection (L=20cm)
A654	Cable assembly LEMO 00 male to MCX male - 1 m
A654 KIT4	4 Cable assembly LEMO 00 male to MCX male - 1 m
A654 KIT8	8 Cable assembly LEMO 00 male to MCX male - 1 m
A659	Cable assembly BNC male to MCX male - 1 m
A659 KIT4	4 MCX TO BNC Cable Adapter
A659 KIT8	8 MCX TO BNC Cable Adapter
AI2730	Optical Fibre 30 m simplex
AI2720	Optical Fibre 20 m simplex
AI2705	Optical Fibre 5 m simplex
AI2703	Optical Fibre 30 cm simplex
AY2730	Optical Fibre 30 m duplex
AY2720	Optical Fibre 20 m duplex
AY2705	Optical Fibre 5 m duplex (RoHS compliant)

**Tab. 1.1:** Table of models and related items.

## 2 Block Diagram

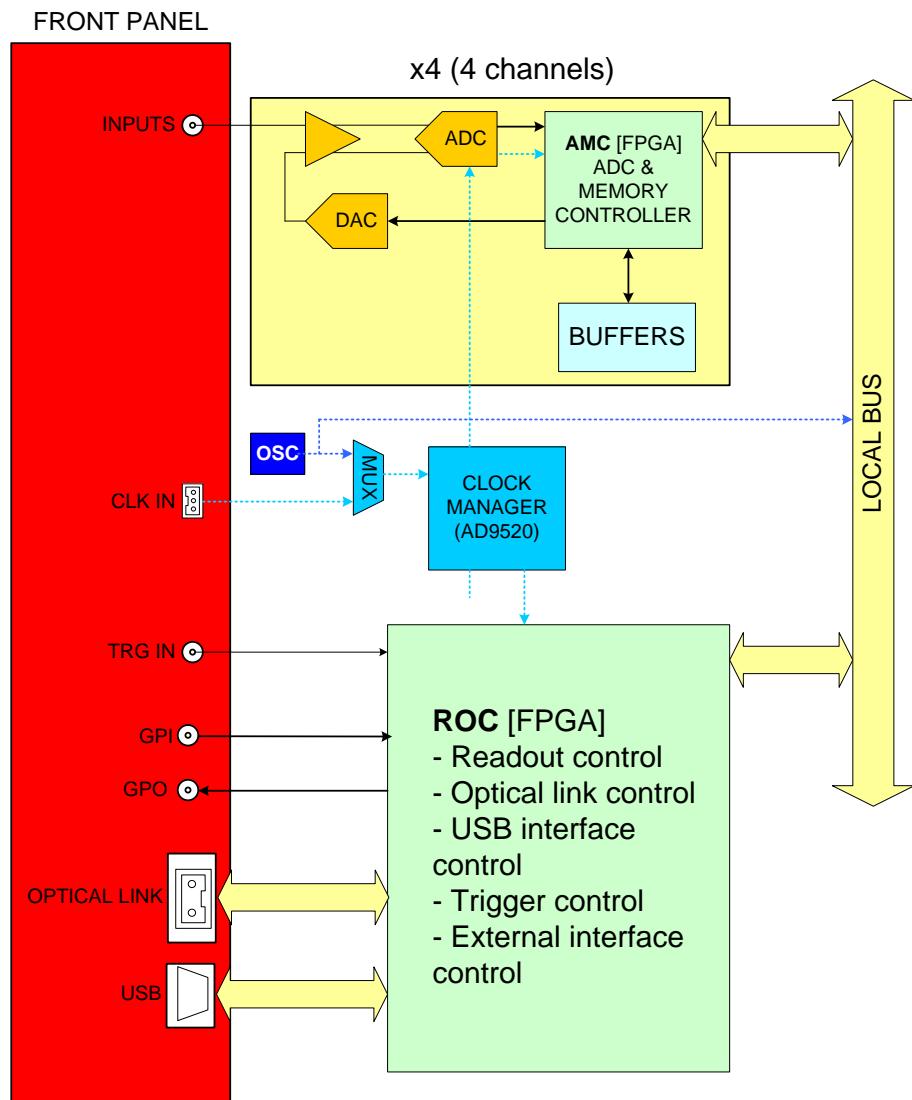


Fig. 2.1: Block Diagram.

### 3 Technical Specifications

<b>ANALOG INPUTS</b>	<p><b>Number of Channels</b></p> <ul style="list-style-type: none"> <li>4 channels/2 channels in DES mode (EVEN channels must be disconnected)</li> <li>Single ended</li> </ul> <p><b>Full Scale Range (FSR)</b> 1 V<sub>pp</sub> or customizable to 200 mV<sub>pp</sub></p>	<p><b>Absolute Max Rating</b></p> <p>@1V<sub>pp</sub>: 3 V<sub>pp</sub> (with V<sub>rail</sub> max +3 V or -3 V for any DAC offset value)</p> <p>@200 mV<sub>pp</sub>: 2 V<sub>pp</sub> (with V<sub>rail</sub> max +2 V or -2 V for any DAC offset value)</p> <p><b>Impedance</b> Z<sub>in</sub> = 50 Ω</p>	<p><b>DC Offset</b> Programmable DAC for DC offset adjustment on each channel in the full range</p> <p><b>Connector</b> MCX</p> <p><b>Bandwidth</b> 500 MHz</p>
<b>DIGITAL CONVERSION</b>	<b>Resolution</b> 10 bits	<b>Sampling Rate</b> 1 GS/s (2 GS/s DES mode) simultaneously on each channel	
<b>SYSTEM PERFORMANCES</b>	ENOB: 9.04 (56 kS Buffer) SINAD: 56.19 dB THD: 70.2 dB SFDR: 79.7 dB SIGMA: 0.58 LSB rms (56 kS buffer, open input)		
<b>FPGA</b>	Two Altera Cyclone EP3C16 (one FPGA serves 2 channels)		
<b>TRIGGER</b>	<p><b>Trigger Source</b></p> <ul style="list-style-type: none"> <li><i>Self-trigger</i>: channel over/under-threshold for common (waveform recording firmware) or individual (DPP firmware only) trigger generation</li> <li><i>External-trigger</i>: common trigger by TRG IN connector or individual by LVDS connector (DPP firmware only)</li> <li><i>Software-trigger</i>: common trigger by software command</li> </ul> <p><b>Trigger Propagation</b> GPO programmable digital output</p>	<p><b>Trigger Time Stamp</b></p> <p><i>Waveform recording FW/DPP-ZLEplus</i>:</p> <ul style="list-style-type: none"> <li>31-bit counter</li> <li>16 ns resolution</li> <li>17 s range</li> <li>48 bit fw extension;</li> </ul> <p><i>DPP-PSD</i>:</p> <ul style="list-style-type: none"> <li>32-bit counter</li> <li>1 ns resolution (1 ps fine time stamp resolution with dCFD)</li> <li>4 s range</li> <li>48 bit fw extension</li> <li>64 bit sw extension;</li> </ul>	
<b>ACQUISITION MEMORY</b>	<p>1.835 MS/ch (3.6 MS/ch in DES mode) or 14.4 MS/ch (28.8 MS/ch in DES mode) (see <b>Tab. 1.1</b>)</p> <p>Multi Event Buffer divisible into 1 ÷ 1024</p> <p>Independent read and write access</p> <p>Programmable event size and pre/post trigger</p>		
<b>ADC CLOCK GENERATION</b>	<p>Clock source: internal/external</p> <p>On-board programmable PLL provides generation of the main board clocks from an internal (50 MHz local Oscillator) or external (front panel CLK-IN connector) reference</p>		
<b>DIGITAL I/O</b>	<p><b>CLK-IN (AMP Modu II)</b> AC coupled differential input clock LVDS, ECL, PECL, LVPECL, CML (single ended NIM/TTL to differential adapter available by A318 accessory)</p> <p>Accuracy &lt; 100 ppm requested</p> <p><b>TRG-IN (LEMO)</b> External trigger digital input Signal Width &gt; 8 ns NIM/TTL, Z<sub>in</sub> = 50 Ω</p>	<p><b>GPO (LEMO)</b> General purpose digital output NIM/TTL, R<sub>t</sub> = 50 Ω</p> <p><b>GPI (LEMO)</b> SYNC/START General purpose digital input Signal Width &gt; 8 ns NIM/TTL, Z<sub>in</sub> = 50 Ω</p>	

<b>SYNCHRONIZATION</b>	<b>Clock Propagation</b> <i>One-to-many</i> : clock distribution from an external clock source to CLK-IN connector	<b>Trigger Time Stamps Alignment</b> By GPI input connector
<b>COMMUNICATION INTERFACES</b>	<b>Optical Link</b> CAEN CONET proprietary protocol Up to 80 MB/s transfer rate Daisy-chain: it is possible to connect up to 8 or 32 ADC modules to a single Optical Link Controller (respectively A2818 or A3818)	<b>USB</b> USB 2.0 compliant Up to 30 MB/s transfer rate
<b>FIRMWARE</b>	<b>Waveform Recording</b> <b>Firmware</b> Free firmware for waveform recording	<b>DPP Firmware</b> DPP-PSD for the Pulse Shape Discrimination DPP-ZLEplus for the Zero Length Encoding
<b>SOFTWARE</b>	<b>Readout SW</b> CAEN software for users and developers: WaveDump, CAENScope, CoMPASS (Windows®, Linux®)	<b>Libraries and Tools</b> General purpose C libraries with readout demos (Windows®, Linux® and LabVIEW™ support) and configuration tools
<b>MECHANICAL</b>	<b>Form Factor</b> Desktop	<b>Weight</b> 675 g
<b>ENVIRONMENTAL</b>	<b>Environment:</b> <b>Operating Temperature:</b> <b>Storage Temperature:</b> <b>Operating Humidity:</b> <b>Storage Humidity:</b> <b>Altitude:</b> <b>Pollution Degree:</b> <b>Overshoot Category:</b> <b>EMC Environment:</b> <b>IP Degree:</b>	Indoor use 0°C to +40°C -10°C to +60°C 10% to 90% RH non condensing 5% to 90% RH non condensing < 2000m 2 II Commercial and light industrial IPX0 Enclosure, not for wet location
<b>REGULATORY COMPLIANCE</b>	<b>EMC</b> CE 2014/30/EU Electromagnetic compatibility Directive	<b>Safety</b> CE 2014/35/EU Low Voltage Directive
<b>POWER CONSUMPTIONS</b>	1.8A @ +12V (Typ.)	

**Tab. 3.1:** Specification table.

## 4 Packaging and Compliancy

The DT5751 digitizer is available as Desktop module housed in a metal case and two external stand up rubber frames (weight: 675 g), one on the front and one on the rear panel (module dimensions: 154 × 50 × 164 mm<sup>3</sup> (WxHxD) excluding the connectors).

The device is inspected by CAEN before the shipment, and it is guaranteed to leave the factory free of mechanical or electrical defects.

The content of the delivered package standardly consists of the part list shown in the table below (**Tab. 4.1**).

Part	Description	Qt
	DT5751 4 Channel 10 bit 2/1 GS/s Digitizer	x1
	Power supply cable and adapter Standard C13 Power Supply chord L=2MT and AC-DC 12V-45W Adapter	x1
	USB cable USB A to B HI-SPEED cable L=2MT	x1
	Documentation UM3350 - DT5751 User Manual	-

**Tab. 4.1:** Delivered kit content.

**CAUTION:** to manage the product, consult the operating instructions provided.

When receiving the unit, the user is strictly recommended to:

- Inspect containers for damage during shipment. Report any damage to the freight carrier for possible insurance claims.
- Check that all the components received match those listed on the enclosed packing list as in **Tab. 4.1**. (CAEN cannot accept responsibility for missing items unless any discrepancy is promptly notified.)
- Open shipping containers; be careful not to damage contents.
- Inspect contents and report any damage. The inspection should confirm that there is no exterior damage to the unit such as broken knobs or connectors and that the front panel is not scratched or

cracked. Keep all packing material until the inspection has been completed.

- If damage is detected, file a claim with carrier immediately and notify CAEN service (see Chap. 14).
- If equipment must be returned, carefully repack equipment in the original shipping container with original packing materials, if possible. Please contact CAEN service.
- If equipment is not installed when unpacked, place equipment in original shipping container and store in a safe place until ready to install.



**DO NOT SUBJECT THE ITEM TO UNDUE SHOCK OF VIBRATIONS**



**DO NOT BUMP, DROP OR SLIDE SHIPPING CONTAINERS**



**DO NOT LEAVE ITEMS OR SHIPPING CONTAINERS UNSUPERVISED IN AREAS WHERE UNTRAINED PERSONNEL MAY MISHANDLE THE ITEMS**



**USE ONLY ACCESSORIES WHICH MEET THE MANUFACTURER SPECIFICATIONS**

For a correct and safe use of the module, refer to Chap. 6 and 7.

## 5 PID (Product Identifier)

PID is the CAEN product identifier, an incremental number greater than 10000 that is unique for each product<sup>1</sup>. The PID is on a label affixed to the product (Fig. 5.1) and it is even stored in an on-board non-volatile memory readable at bit [7:0] of registers 0xF080 or 0xF084 [RD1]. The PID information is also available through CAENUpgrader Software, with the Get Information function of the GUI (for more details refer to [RD5]).



**Note:** The serial number is still valid to identify older boards, where the PID label is not present.



**Fig. 5.1:** PID location on DT5751 (the number in the picture is purely indicative).

---

<sup>1</sup>The PID substitutes the serial number previously identifying the boards.

## 6 Power Requirements

DT5751 module is powered by the external AC/DC stabilized power supply provided with the digitizer and included in the delivered kit.

The DT5751 typical power consumption is 1.8 A (@ +12 V).



**Note:** Using a different power supply source, like battery or linear type, it is recommended the source to provide +12 V and, at least, 2 A in case of DT5751; the power jack is a 2.1 mm type, a suitable cable is the RS 656-3816 type (or similar)



**Fig. 6.1:** AC/DC power supply provided with the module.

# 7 Cooling Management

The D5751 Digitizer can operate in the temperature range  $0^\circ \div +40^\circ\text{C}$  [RD6].

It is equipped with air flow fans installed onboard, which take care of the proper cooling of the board.



**EXTERNAL FANS MUST BE USED WHEN THE BOARD IS INSTALLED IN A SETUP WITH POOR AIR FLOW**

The User must take care to provide a proper cooling to the board with external fan if the board is used in an enclosure or if the board is installed in a setup with poor air flow.

Excessive temperature will, in first instance, reduce the performance and the quality of the measurements and can also damage the board.

If the board is stored in cold environment, please check for water condensation before power on.

The board has not been tested for radiation hardness. High energy particles can be source of errors and can damage the FPGA. If used in strong proton or neutron beams, arrange proper shielding, or remote the sensors with a custom cable.

## 7.1 ADC chips temperature readout

The V1751 features an internal ADC temperature monitoring system, useful in order to estimate the steady thermal state of the ADCs and to perform the calibration procedure (see Sec. 9.7.1). Since each ADC manages two channels (0-1, 2-3, 4-5, 6-7) identical temperature values will be found for couples of channels; such values can be readout using register 0x1nA8.

## 7.2 ADC chips over temperature protection

Each ADC will be automatically powered off whenever the core temperature reaches  $90^\circ\text{C}$ . The relevant channels will not therefore participate any more to data event, and bit[7] and bit[8] of register 0x1n88 will set to 1 (channel power down and over-temperature flags respectively).

When the ADC core temperature decreases under  $65^\circ\text{C}$ , the bit[8] will return to 0, and the relevant channels can be restored to normal operation following these steps:

- Wait until bit 8 of 0x1n88 register returns to 0
- Set bit[0] = 0 of 0x1n9C; bit[7] of 0x1n88 will return to 0.
- Perform a calibration procedure on the restored channels (see Sec. 9.7.1)

## 7.3 Cleaning Air Vents

CAEN recommends to occasionally clean the air vents on all vented sides of the board or crate, if present. Lint, dust, and other foreign matter can block the vents and limit the airflow. Be sure to power off the

board and disconnect it from the power by physically detach the power chord before cleaning the air vents and follow the general cleaning safety precautions.



**IT IS UNDER THE RESPONSIBILITY OF THE CUSTOMER A  
NON-COMPLIANT USE OF THE PRODUCT**

## 8 Panels Description




Fig. 8.1: Front panel view.



Fig. 8.2: Rear panel view.

## 8.1 Front Panel

ANALOG INPUT		
	<b>FUNCTION</b> Input connectors from CH0 to CH3 receive the input analog signals.  <b>ELECTRICAL Specs</b> Input dynamics: $1 \text{ V}_{\text{pp}}$ Input impedance ( $Z_{\text{in}}$ ): $50 \Omega$ . Absolute max analog input voltage: @ $1\text{V}_{\text{pp}}$ : $3 \text{ V}_{\text{pp}}$ (with $V_{\text{rail}}$ max $+3 \text{ V}$ or $-3 \text{ V}$ ) @ $200 \text{ mV}_{\text{pp}}$ : $2 \text{ V}_{\text{pp}}$ (with $V_{\text{rail}}$ max $+2 \text{ V}$ or $-2 \text{ V}$ ) for any DAC offset value. <b>Note:</b> $200 \text{ (} 50 \Omega \text{)} \text{ mV}_{\text{pp}}$ input range is available by ordering option (see Tab. 1.1).	<b>MECHANICAL Specs</b> Series: MCX connectors. Type: CS 85MCX-50-0-16 (jack/female). Manufacturer: SUHNER Suggested plug/male: MCX-50-2-16 type. Suggested cable: RG174 type.


CLOCK IN		
	<b>FUNCTION</b> Input connector for the external clock.  <b>ELECTRICAL Specs</b> Sign. type: differential (LVDS, ECL, PECL, LVPECL, CML). CAEN provides single ended-to-differential A318 cable adapter (see Tab. 1.1). Coupling: AC (CLK-IN). $Z_{\text{diff}}$ : $100 \Omega$ .	<b>MECHANICAL Specs</b> Series: AMPMODU connectors. Type: 3-102203-4 (3-pin). Manufacturer: AMP Inc. <b>PINOUT</b> 

**CLK IN LED (GREEN):** indicates the external clock is enabled.


GENERAL PURPOSE OUTPUT		
	<b>FUNCTION</b> General purpose programmable digital output connector to propagate: <ul style="list-style-type: none"> <li>the internal trigger sources;</li> <li>the channel probes (i.e. signals from the mezzanines);</li> <li>GPI signal</li> </ul> according to register addresses 0x8110 and 0x811C, or <ul style="list-style-type: none"> <li>the motherboard probes (i.e. signals from the motherboard), like the Run signal, ClkOut signal, ClockPhase signal, PLL_Unlock signal or Busy signal</li> </ul> according to register address 0x811C.  <b>ELECTRICAL Specs</b> Signal level: NIM or TTL. Requires $50 \Omega$ termination.	<b>MECHANICAL Specs</b> Series: 101 A 004 connectors. Type: DLP 101 A 004-28. Manufacturer: FISCHER. <b>Alternatively:</b> Type: EPL 00 250 NTN. Manufacturer: LEMO.

TRG-IN			
	<b>FUNCTION</b> Digital input connector for the external trigger.  <b>ELECTRICAL Specs</b> Signal level: NIM or TTL. Input impedance ( $Z_{in}$ ): 50 Ω.	<b>MECHANICAL Specs</b> Series: 101 A 004 connectors. Type: DLP 101 A 004-28. Manufacturer: FISCHER. <b>Alternatively:</b> Type: EPL 00 250 NTN. Manufacturer: LEMO.	

GENERAL PURPOSE INPUT			
	<b>FUNCTION</b> General purpose programmable input connector. Can be used to reset the time stamp (see <b>Sec. Reset, Clear and Default Configuration</b> ) or to start/stop the acquisition.  <b>ELECTRICAL Specs</b> Signal level: NIM or TTL. Input impedance ( $Z_{in}$ ): 50 Ω.	<b>MECHANICAL Specs</b> Series: 101 A 004 connectors. Type: DLP 101 A 004-28. Manufacturer: FISCHER. <b>Alternatively:</b> Type: EPL 00 250 NTN. Manufacturer: LEMO.	

OPTICAL LINK PORT			
	<b>FUNCTION</b> Optical LINK connector for data readout and flow control. Daisy chainable. Compliant with Multimode 62.5/125 μm cable featuring LC connectors on both sides.  <b>ELECTRICAL Specs</b> Transfer rate: up to 80 MB/s.	<b>MECHANICAL Specs</b> Series: SFF Transceivers. Type: FTLF8519F-2KNL (LC connectors). Manufacturer: FINISAR.	<b>PINOUT</b>  TX RX

**LINK LEDs (GREEN/YELLOW):** right LED (GREEN) indicates the network presence, while left LED (YELLOW) signals the data transfer activity.

USB PORT			
	<b>FUNCTION</b> USB connector for data readout and flow control.  <b>ELECTRICAL Specs</b> Standard: compliant with USB 2.0 and USB 1.0. Transfer rate: up to 30 MB/s.	<b>MECHANICAL Specs</b> Series: USB connectors. Type: 787780-2 (B-Type). Manufacturer: AMP Inc.	

**USB LINK LED (GREEN):** indicates the USB communication is active.

DIAGNOSTICS LEDs	
	<p><b>TTL (GREEN)</b>: indicates that the standard TTL is set for GPO, TRG IN, GPI;</p> <p><b>NIM (GREEN)</b>: indicates that the standard NIM is set for GPO, TRG IN, GPI;</p> <p><b>DTACK (GREEN)</b>: indicates there is a read/write access to the board;</p> <p><b>PLL LOCK (GREEN)</b>: indicates the PLL is locked to the reference clock;</p> <p><b>PLL BYPS (GREEN)</b>: not used;</p> <p><b>RUN (GREEN)</b>: indicates the acquisition is running (data taking). See Sec. 9.7.2;</p> <p><b>TRG (GREEN)</b>: indicates the trigger is accepted;</p> <p><b>RDY (GREEN)</b>: indicates the event/data is present in the Output Buffer;</p> <p><b>BUSY (RED)</b>: indicates all the buffers are full for at least one channel.</p>

## 8.2 Rear Panel

SPARE LINK	
	<p><b>FUNCTION</b> Auxiliary connector reserved for CAEN usage.</p> <p><b>ELECTRICAL Specs</b> N/A</p> <p><b>MECHANICAL Specs</b> Series: Header connectors. Type: 7610-5002-5+5. Manufacturer: 3M.</p>

DC INPUT	
	<p><b>FUNCTION</b> Input connector for the desktop Digitizer main power supply from the external AC/DC adapter.</p> <p><b>ELECTRICAL Specs</b> Typ. Input voltage: +12 VDC.</p> <p><b>MECHANICAL Specs</b> Series: CC power supply connectors Type: RAPC722X (DC power jack). Manufacturer: Switchcraft Inc.</p> <p><b>PINOUT</b> </p>

ON/OFF SWITCH	
	<p><b>DESCRIPTION</b> On/off switch.</p> <p><b>FUNCTION</b> Switch ON or OFF the module power supply: O → power supply OFF;   → power supply ON.</p> <p><b>ELECTRICAL Specs</b> N/A</p> <p><b>MECHANICAL Specs</b> Series: A1 switches. Type: A11332211000 (single-pole, two-way). Manufacturer: Molveno.</p>

IDENTIFICATION LABELS	
	<p><b>FUNCTION</b> Reports:</p> <ul style="list-style-type: none"> <li>• Board model and input dynamic range (default)</li> <li>• CE conformity marking</li> <li>• PID barcode</li> <li>• PID number</li> </ul>

# 9 Functional Description

## 9.1 Analog Input Stage

Input dynamic is  $1 \text{ V}_{\text{pp}}$ ;  $200 \text{ mV}_{\text{pp}}$  version is available upon request (see **Tab. 1.1**). In order to preserve the full dynamic range with unipolar input signal, positive or negative, it is possible to add a DC offset by means of a 16 bit DAC, which is up to  $\pm 0.5 \text{ V}$  @  $1 \text{ V}_{\text{pp}}$  and  $\pm 0.1 \text{ V}$  @  $200 \text{ mV}_{\text{pp}}$ . The input bandwidth ranges from DC to 500 MHz (with 2<sup>nd</sup> order linear phase anti-aliasing low pass filter).

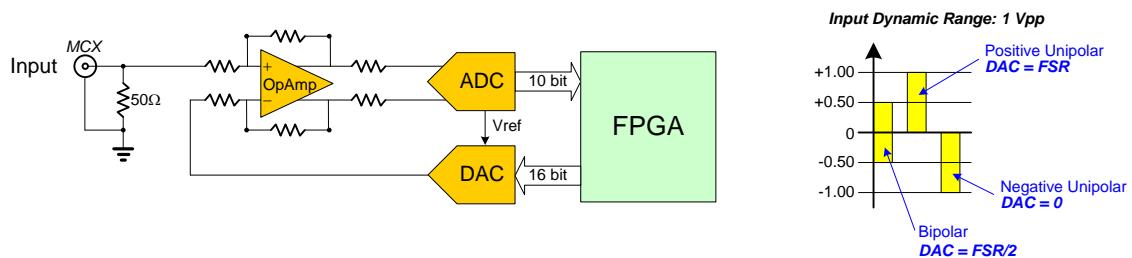


Fig. 9.1: Analog input diagram.

### 9.1.1 DC Offset Individual Setting

Setting the DC offset for channel n requires a write access at register addresses 0x1n98. Writing at 0x8098, the DC offset will apply to all channels at once. Refer to **[RD1]** for more details.

## 9.2 Clock Distribution

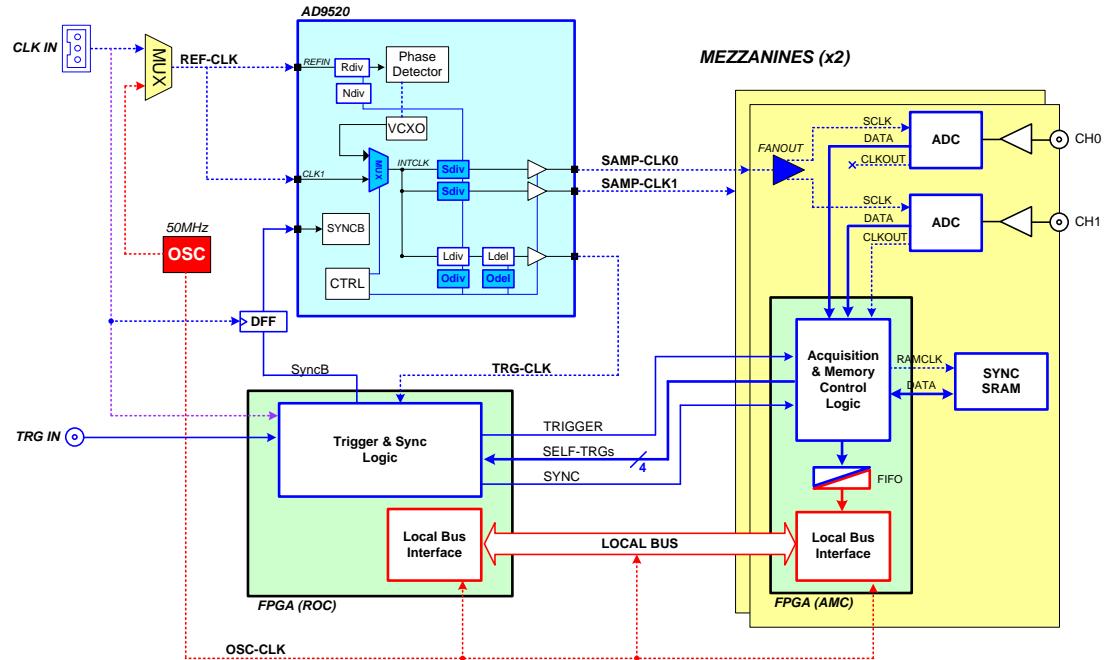


Fig. 9.2: Clock distribution diagram.

The clock distribution of the module takes place on two domains: OSC-CLK and REF-CLK.

OSC-CLK is a fixed 50-MHz clock coming from a local oscillator which handles USB, Optical Link and Local Bus, that takes care of the communication between motherboard and mezzanines (see red traces in Fig. 9.2).

REF-CLK handles ADC sampling, trigger logic, and acquisition logic (samples storage into RAM, buffer freezing on trigger) through a clock chain. REF-CLK can be either an external (via the front panel CLK-IN connector) or an internal (via the 50-MHz local oscillator) source. In the latter mode, OSC-CLK and REF-CLK will be synchronous (the operation mode remains the same).

REF-CLK clock source selection can be done by writing bit[6] of register 0x8100 [RD1] between the following modes:

- INT mode (default) means REF-CLK is the 50 MHz of the local oscillator (REF-CLK = OSC-CLK);
- EXT mode means REF-CLK source is the external frequency fed on CLK-IN connector.

The external clock signal must be differential (LVDS, ECL, PECL, LVPECL, CML) with a jitter lower than 100 ppm (see Chap. 3). CAEN provides the A318 cable to adapt single ended signals coming from an external clock unit into the differential CLK-IN connector (see Tab. 1.1).

The DT5751 is equipped with a phase-locked-loop (PLL) and clock distribution device, AD9520. It receives the REF-CLK and generates the sampling clock for ADCs and the mezzanine FPGA (SAMP-CLK0 and SAMP-CLK1), as well as the trigger logic synchronization clock (TRG-CLK) and the output clock (CLK-OUT).

AD9520 configuration can be changed and stored into non-volatile memory. Changing the AD9520 configuration is primarily intended to be used for external PLL reference clock frequency change (see Sec. 9.3). The DT5751 locks to an external 50 MHz reference clock with default AD9520 configuration.

Refer to the AD9520 datasheet [RD7] for more details.

## 9.3 PLL Mode

The Phase Detector within the AD9520 device allows to couple REF-CLK with an internal VCXO, which provides the nominal ADCs frequency (1 GS/s).

As introduced in Sec. 9.2, the source of the REF-CLK signal (see Fig. 9.2) can be external on CLK-IN front panel connector or internal from the 50 MHz local oscillator.

The following options are allowed:

1. 50 MHz internal clock source - this is the standard operation mode: the AD9520 dividers do not require to be reprogrammed (the digitizer works in the AD9520 default configuration). The clock source selection bit (bit[6] of 0x8100 **[RD1]**) is in default INT mode. REF-CLK = OSC-CLK.
2. 50 MHz external clock source - in this case, the clock source is taken from an external device; the AD9520 dividers do not need to be reprogrammed as the external frequency is the same as the default one. The clock source selection bit (bit[6] of 0x8100 **[RD1]**) must be set in EXT mode. CLK-IN = REF-CLK = OSC-CLK.
3. External clock source different from 50 MHz - the clock source is externally provided as in point 2, but the AD9520 dividers must now be reprogrammed to lock the the VCXO to the new REF-CLK in order to provide out the nominal sampling frequency at 1 GS/s. The clock source selection bit (bit[6] of 0x8100 **[RD1]**) must be set in EXT mode. CLK-IN = REF-CLK  $\neq$  OSC-CLK.

If the digitizer is locked, the PLL-LOCK front panel LED must be on.



**Note:** The user who wants to work as in point 3, please contact CAEN (see Chap. 14) indicating the required reference clock frequency, to check its feasibility and then receive the PLL programming file. The “Upgrade PLL” function in CAENUpgrader software tool can be used to update the digitizer PLL **[RD5]**.

## 9.4 Reducing the Sampling Frequency

In case the board is required to work at a sampling frequency (SAMP-CLK) lower than the nominal, it can be achieved by reprogramming the AD9520 dividers. REF-CLK can be configured as in Sec. 9.3. Not all the frequencies are admitted and a lower frequency limit must be considered, due to the internal electronics. Please contact CAEN (see Sec. 14) to check the feasibility.



**Note:** The mimimum sampling frequency by hardware downsampling is 250 MS/s **[RD8]**.

## 9.5 Trigger Clock

The TRG-CLK logic works at 125 MHz, equal to 1/8 of the sampling frequency: TRG-CLK = 1/8 · SAMPL-CLK. Eight samples of trigger “uncertainty” occurs over the acquisition window (16 samples uncertainty in DES mode).

## 9.6 DES Mode

The board can be programmed to operate in Dual Edge Sampling (DES) mode, at 2 GS/s.

DES Mode is configurable by setting bit[12] = 1 of register 0x8000 (see **[RD1]**).



**Note:** Only even channels are managed when operating the digitizer in DES mode.




**Note:** DES mode is not available in case of DPP-PSD firmware usage.

## 9.7 Acquisition Modes

### 9.7.1 Channel Calibration

The module performs a self-calibration of the ADCs at its power-on. Anyway, in order to achieve the best performance, the calibration procedure is recommended to be executed by the user, on command, after the ADCs have stabilized their operating temperature. The calibration will not need to be repeated at each run unless the operating temperature changes significantly, or clock settings are modified (e.g. switching from internal to external clock).

The diagram below synthesises the flow for a proper calibration:

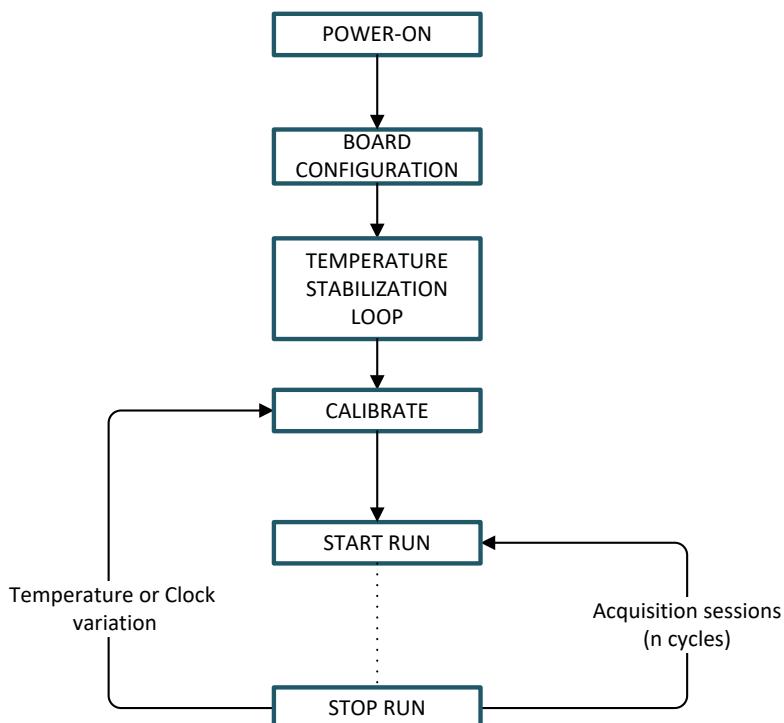

**Fig. 9.3:** Diagram of the ADC calibration flow.

- At low level, the ADCs temperature can be read at the register address 0x1nA8 [RD1], while the calibration must be performed through register address 0x809C. The following steps are required:
  - set bit[1] = 0 of register 0x809C;
  - set bit[1] = 1 of register 0x809C. The self calibration process will start simultaneously on each channel of the board and bit[6] of register 0x1n88 will be set to 0;
  - poll bit[6] of register 0x1n88 until it returns to 1 (few milliseconds);

- set again bit[1] = 0 of register 0x809C.

Steps in case of DES mode are:

- make sure that EVEN channels are disconnected;
- disable EVEN channels;
- enable DES mode by setting bit[12] = 1 of register 0x8000;
- set bit[1] = 0 of register 0x809C;
- set bit[1] = 1 of register 0x809C. The self calibration process will start simultaneously on each channel of the board and bit[6] of register 0x1n88 will be set to 0;
- poll bit[6] of register 0x1n88 until it returns to 1 (few milliseconds);
- set again bit[1] = 0 of register 0x809C.



**Note:** Whenever switching from Normal mode to DES mode and vice-versa, the ADC calibration must be repeated.



**Note:** It is normally not required to calibrate after a board reset but, if a Reset command is intentionally issued to the digitizer (write access at register address 0xEF24) to be directly followed by a calibration procedure, it is recommended to wait for the board to reach stable conditions (indicatedly 100 ms) before starting the calibration.



**Note:** At power-on, a Sync command is also issued by the firmware to the ADCs to synchronize all of them to the board's clock. In the standard operating, this command is not required to be repeated by the user. If a Sync command is intentionally issued (write access at register address 0x813C), the user must consider that a new calibration procedure is needed for a correct board operating.

- At the library level, developers can exploit the CAENDigitizer library (see Sec. 10.2) dedicated routines which are *ReadTemperature()* function for temperature readings and the *Calibrate()* function which executes the channel calibration steps above described.



**Note:** Starting from CAENDigitizer release 2.6.1, the *Reset()* function has been modified so that it no longer includes the channel calibration routine implemented in the code. This calibration must be performed on command by the dedicated *Calibrate()* function. Please, see the Library user manual for reference ([RD9]).

- At software level, CAEN manages the command channel calibration in different readout software (please, refer the relevant software User Manual [RD10] and [RD2] for details).

◊ **WaveDump**

1. Launch WaveDump. This software performs an automatic ADC calibration and displays a message when it is completed (see Fig. 9.4). This allows the user to start using the program sure

```
*****
* Wave Dump 3.7.2.20160420
*****
Opening Configuration File WaveDumpConfig.txt
Connected to CAEN Digitizer Model DT5751
ROC FPGA Release is 04.00 - Build 0401
AMC FPGA Release is 00.06 - Build 0401
ADC Calibration successfully executed.
[ls] start/stop the acquisition, [q] quit, [SPACE] help
-
```

**Fig. 9.4:** Automatic calibration at WaveDump first run.

that the digitizer has been calibrated at least once.

**NOTE THAT: If SKIP\_STARTUP\_CALIBRATION parameter is set to YES in WaveDump configuration file, the automatic start-up calibration is not performed and no message is displayed**

2. At any time, the user can check the channel temperatures (with the acquisition not running) by issuing multiple “m” commands from the keyboard.
3. In case of significant variations, issuing a “c” command provokes a manual channel calibration to be executed (see **Fig. 9.5**).

```

Reading at 4.49 MB/s (Trg Rate: 1137.62 Hz)
Reading at 4.47 MB/s (Trg Rate: 1133.66 Hz)
Acquisition stopped
CH00: 31 C
CH01: 31 C
CH02: 31 C
CH03: 31 C
CH04: 28 C
CH05: 28 C
CH06: 28 C
CH07: 28 C

CH00: 31 C
CH01: 31 C
CH02: 31 C
CH03: 31 C
CH04: 29 C
CH05: 29 C
CH06: 29 C
CH07: 29 C

ADC Calibration successfully executed.

```


**Fig. 9.5:** Temperature monitoring with manual calibration in WaveDump software.

4. A new acquisition can start.

Please, refer to WaveDump User Manual for complete software description **[RD10]**.

◊ **CoMPASS**

1. Launch CoMPASS Software
2. Connect to the digitizer
3. Before to start the acquisition, go to the “Input” tab and enable “Calib.ADC” checkcell.
4. Start the acquisition: the calibration of the channel ADCs is performed at every start acquisition.

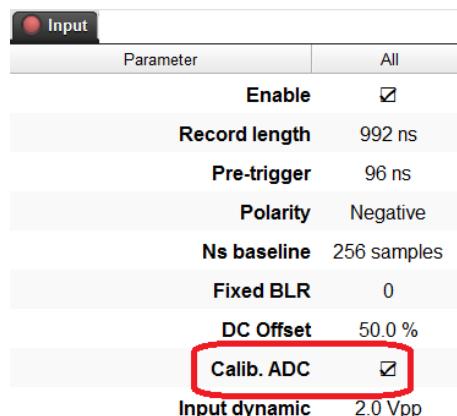

**Fig. 9.6:** Channel calibration in CoMPASS Software.

## 9.7.2 Acquisition Run/Stop

The acquisition can be started and stopped in different ways, according to bits[2:0] of register 0x8100 **[RD1]**:

- SW CONTROLLED (bits[1:0] = 00): Start and Stop take place by software command. Bit[2] = 0 means stopped, while bit[2] = 1 means running.
- GPI CONTROLLED (bits[1:0] = 01): acquisition is armed by setting bit[2] = 1, the two options are selectable through bit[11] of the same register:
  - START/STOP ON LEVEL - If bit[11] = 0, then acquisition starts when the GPI signal is high and stops when it is low; if bit[2] = 0 (disarmed), the acquisition is always off.
  - START ON EDGE - If bit[11] = 1, then acquisition starts on the rising edge of the GPI signal and must be stopped by software command (bit[2] = 0).



**Note:** the START ON EDGE option is implemented from ROC FPGA fw revision 4.22 on.

- FIRST TRIGGER CONTROLLED (bits[1:0] = 10): bit[2] = 1 arms the acquisition and the Start is issued on the first trigger pulse (rising edge) on the TRG-IN connector. This pulse is not used as a trigger; actual triggers start from the second pulse on TRG-IN. The Stop acquisition must be SW controlled (i.e. reset of bit[2]).

## 9.7.3 Acquisition Triggering: Samples and Events

When the acquisition is running, a trigger signal allows to:

- store a 31-bit counter value of the Trigger Time Tag (TTT).  
The counter (representing a time reference), like the Trigger Logic Unit (see **Fig. 9.2**), operates at a frequency of 125 MHz (i.e. 8 ns, that is to say 8 ADC clock cycles). Due to the way acquired data is written into the board internal memory (i.e. in 4-sample bunches), the TTT counter is read every 2 trigger logic clock cycles, which means the trigger time stamp resolution results in 16 ns (i.e. 62.5 MHz). Basing on that, the LSB of the TTT is always "0";
- increment the EVENT COUNTER;
- fill the active buffer with the pre/post-trigger samples, whose number is programmable via register address 0x8114 **[RD1]**; the acquisition window width (also referred to as record length) is determined via register addresses 0x800C and 0x8020; then, the buffer is frozen for readout purposes, while the acquisition continues on another buffer.

An event is therefore composed by the trigger time tag, pre- and post-trigger samples and the event counter.

Overlap between "acquisition windows" may occur (a new trigger occurs while the board is still storing the samples related to the previous trigger); this overlap can be either rejected or accepted (programmable via software by writing at register address 0x8000 **[RD1]**).

If the board is programmed to accept the overlapping triggers, as soon as the "overlapping" trigger arrives, the current active buffer is filled up, then the samples storage continues on the subsequent one. In this case, not all events will have the same size (see **Fig. 9.7**).

A trigger can be refused for the following causes:

- Acquisition is not active.
- Memory is FULL and therefore there are no available buffers.
- The required number of samples for building the event pre-trigger is not reached yet; this happens typically as the trigger occurs too early either with respect to the RUN Acquisition command (see **Sec. 9.7.2**) or with respect to a buffer emptying after a Memory FULL status (see **Sec. 9.7.6**).

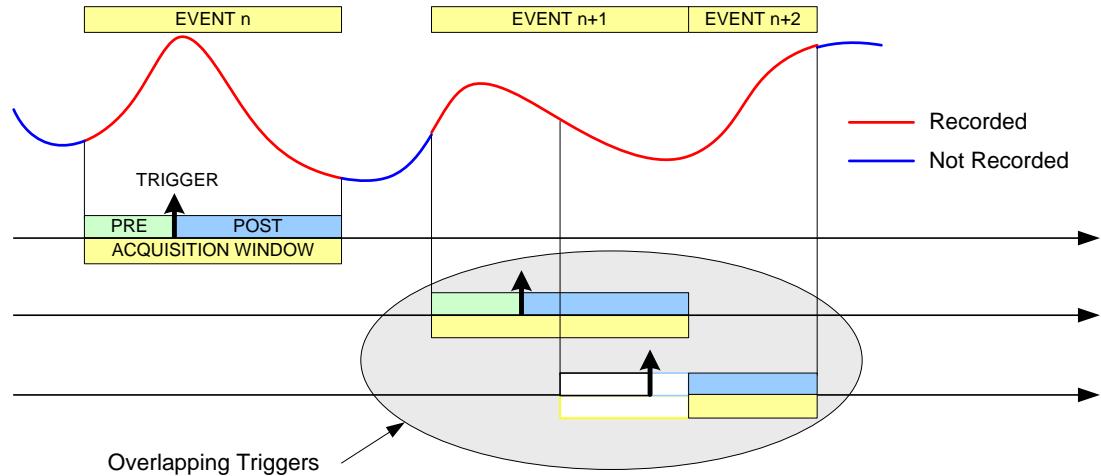


Fig. 9.7: Trigger Overlap.

- The trigger overlaps the previous one and the board is not enabled for accepting overlapped triggers.

As a trigger is refused, the current buffer is not frozen and the acquisition continues writing on it. The EVENT COUNTER can be programmed in order to be either incremented or not. If this function is enabled, the EVENT COUNTER value identifies the trigger number sent (but the event number sequence is lost); if the function is not enabled, the EVENT COUNTER value coincides with the sequence of buffers saved and readout.

## 9.7.4 Multi-Event Memory Organization

Each channel of the DT5751 features a SRAM memory to store the acquired events. The memory size in the standard event storage mode is 1.75 MS or 13.73 MS<sup>1</sup>, where  $M = 1024 \cdot 1024$ , according to the board version (see Tab . 1.1). The channel memory can be divided in a programmable number of buffers,  $N_b$  ( $N_b$  from 1 up to 1024), by the register address 0x800C [RD1], as described in Tab. 9.1.



**Note:** in case of DES mode, values must be multiplied by 2.

Register Value BUFFER_CODE	Number of Buffers ( $N_b$ )	Size of one Buffer	
		SRAM 2.33 MB/ch (1.75 MS)	SRAM 18.3 MB/ch (13.73 MS)
0x00	1	2.333 MB/ch (1.75 MS)	18.3 MB/ch (13.73 MS)
0x01	2	1.167 MB/ch (896 kS)	9.1 MB/ch (6.8 MS)
0x02	4	597.2 kB/ch (448 kS)	4.6 MB (3.4 MS)
0x03	8	298.6 kB/ch (224 kS)	2.3 MB/ch (1.7 MS)
0x04	16	149.3 kB/ch (112 kS)	1.1 MB/ch (878.7 kS)
0x05	32	74.6 kB/ch (56 kS)	586.2 kB/ch (439.3 kS)
0x06	64	37.3 kB/ch (28 kS)	293.1 kB/ch (219.7 kS)
0x07	128	18.7 kB/ch (14 kS)	146.6 kB/ch (109.8 kS)
0x08	256	9.3 kB/ch (7 kS)	73.3 kB/ch (54.9 kS)
0x09	512	4.7 kB/ch (3.5 kS)	36.6 kB/ch (27.4 kS)
0x0A	1024	2.3 kB/ch (1.75 kS)	18.3 kB/ch (13.7 kS)

**Tab. 9.1:** Buffer organization of 751 family series. For each value of buffer size it is reported the memory size and the number of samples of one buffer, where  $k = 1024$  and  $M = 1024 \cdot 1024$ .

Having 1.75 MS memory size as reference, this means that each buffer contains  $1.75M/N_b$  samples (e.g.  $N_b = 1024$  means 1.75k samples in each buffer).

### 9.7.4.1 Custom size events

In case an event size less than the buffer size is needed, the user can set the  $N_{LOC}$  value at register address 0x8020 [RD1], where  $N_{LOC}$  is the number of memory locations. The size of the event is so forced to be according to the formula:

$$1 \cdot N_{LOC} = 7 \cdot N_{Sample} \text{ (normal mode)}$$

$$1 \cdot N_{LOC} = 14 \cdot N_{Sample} \text{ (DES mode)}$$

When  $N_{LOC} = 0$  the custom size is disabled.



**Note:** The value of  $N_{LOC}$  must be set in order that the relevant number of samples does not exceed the buffer size and it must not be modified while the acquisition is running. Even using the custom size setting, the number of buffers and the buffer size are not affected by  $N_{LOC}$ , but they are still determined by  $N_b$ .

The concepts of buffer organization and custom size directly affect the width of the acquisition window (i.e. number of the digitized waveform samples per event). The Record Length parameter defined in CAEN software (such as WaveDump and CAENScope introduced in Chap. 11) and the `Set/GetRecordLength()` functions of the CAENDigitizer library rely on these concepts [RD9].

<sup>1</sup>Memory size is 1.8 MS and 14.4 MS in case of  $M = 1000 \cdot 1000$ .

## 9.7.5 Event structure

The event can be readout via USB or Optical Link; data format is 32-bit long word (see [Fig. 9.10](#)).

An event is structured as:

- **Header** (four 32-bit words)
- **Data** (variable size and format)

### 9.7.5.1 Header

The Header consists of four words including the following information:

- **EVENT SIZE** (bits[27:0] of 1<sup>st</sup> header word) is the total size of the event, i.e. the number of 32-bit long words to be read.
- **BOARD FAIL FLAG** (bit[26] of 2<sup>nd</sup> header word) implemented from ROC FPGA firmware revision 4.5 on (reserved otherwise), it is set to “1” in consequence of a hardware problem (e.g. PLL unlocking). The user can collect more information about the cause by reading at register address 0x8178 and contact CAEN Support Service if necessary (see [Chap. 14](#)).
- **TRG OPTIONS** (bits[23:8] of 2<sup>nd</sup> header word); starting from revision **4.6** of the ROC FPGA firmware (reserved otherwise), these 16 bits can be programmed to provide trigger information according to the setting of the bits[22:21] at register address 0x811C (see [Tab 9.2](#)).

REGISTER 0x811C Bits[22:21]	FUNCTIONAL DESCRIPTION	Reserved / TRG OPTIONS INFORMATION (bit[23:8] of 2 <sup>nd</sup> header word)
00 (default)	Reserved	Must be 0
01	Event Trigger Source	Indicates the trigger source causing the event acquisition: Bits[23:19] = 00000 Bit[18] = Software Trigger Bit[17] = External Trigger Bit[16:12] = 000000 Bits[11:8] = Channel self-trigger (refer to <a href="#">Sec. 9.8.3</a> )
10	Extended Trigger Time Tag (ETTT)	A 48-bit Trigger Time Tag (ETTT) information is configured, where Bits[23:8] contributes as the 16 most significant bits together to the 32-bit TTT field (4 <sup>th</sup> header word) <b>Note:</b> in the ETTT option, the overflow bit is not provided
11	Not used	If configured, it acts like “00” setting

**Tab. 9.2:** Reserved/Trg Options configuration table.

- **CHANNEL MASK** (bits[3:0] of 2<sup>nd</sup> header word) is the mask of the channels participating in the event (e.g. CH0 and CH2 participating → Channel Mask = 0x5). This information must be used by the software to acknowledge from which channel the samples are coming (the first event contains the samples from the channel with the lowest number).



**Note:** in DES mode even channels are automatically disabled.

- **EVENT COUNTER** (bits[23:0] of 3<sup>rd</sup> header word) is the trigger counter; it can count either accepted triggers only, or all triggers (bit[3] of register address 0x8100).
- **TRIGGER TIME TAG** (bits[31:0] of 4<sup>th</sup> header word) is the 31-bit Trigger Time Tag (TTT) information, which is the trigger time reference (see Sec. 9.7.3). The word is composed of the value of the 31-bit counter of the Trigger Time Tag (bit[30:0]) plus the overflow bit (bit[31]) indicating that the timestamp counter has overflowed at least once (Fig. 9.8). If the ETTT option is enabled, then this field becomes the 32 less significant bits of the 48-bit Extended Trigger Time Tag information in addition to the 16 bits (MSB) of the TRG OPTIONS field (2<sup>nd</sup> event word). Note that, in the ETTT case, the overflow bit is no more provided (Fig. 9.9). The trigger time tag is reset either at the start of acquisition, or via front panel signal on S-IN or LVDS I/O connectors, and increments with 250 MHz frequency (i.e. every 8 ADC clock cycles). The TTT value is read at half the frequency (i.e. 125 MHz) so that the specifications are 16 ns resolution and 17 s range ( $8 \text{ ns} \times (2^{31} - 1)$ ), which can be extended to 625 h ( $8 \text{ ns} \times (2^{48} - 1)$ ) if ETTT is enabled.

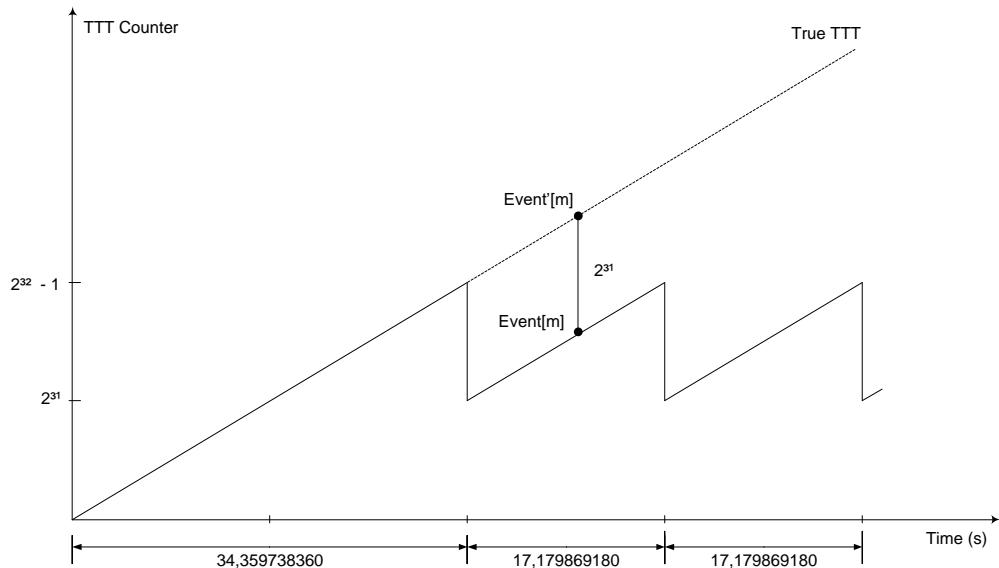


Fig. 9.8: TTT description.

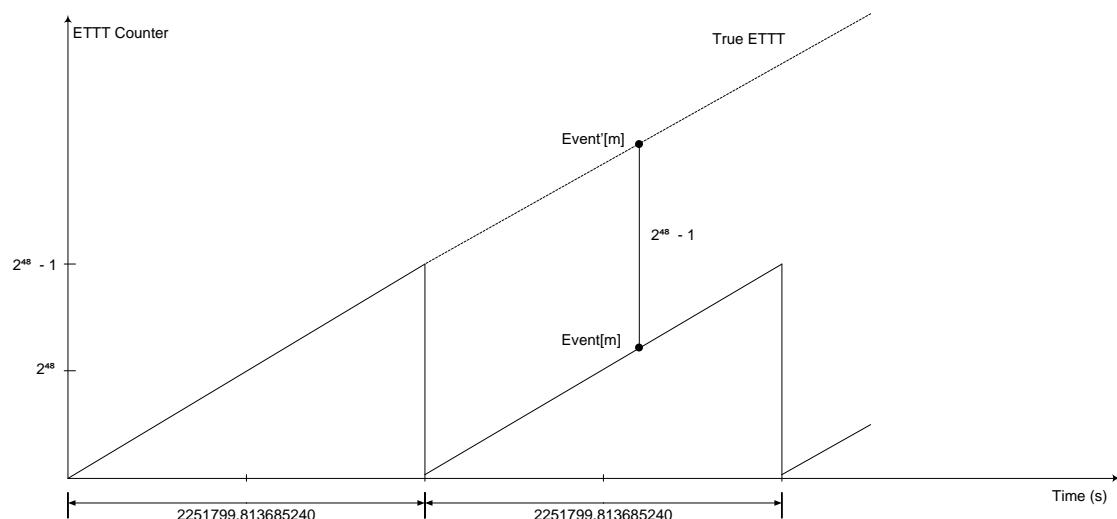


Fig. 9.9: ETTT description.

### 9.7.5.2 Data

Data are the stored samples. Data from masked channels are not read. When operating in DES mode the EVEN channels are automatically disabled. Bits[31:30] of the data words identifies how many samples are stored in the corresponding word. The example in Sec. 9.7.5.3 shows the case of two samples in the last word.

### 9.7.5.3 Event Format Examples

The event format is shown in the following figure (case of 4 channels enabled):

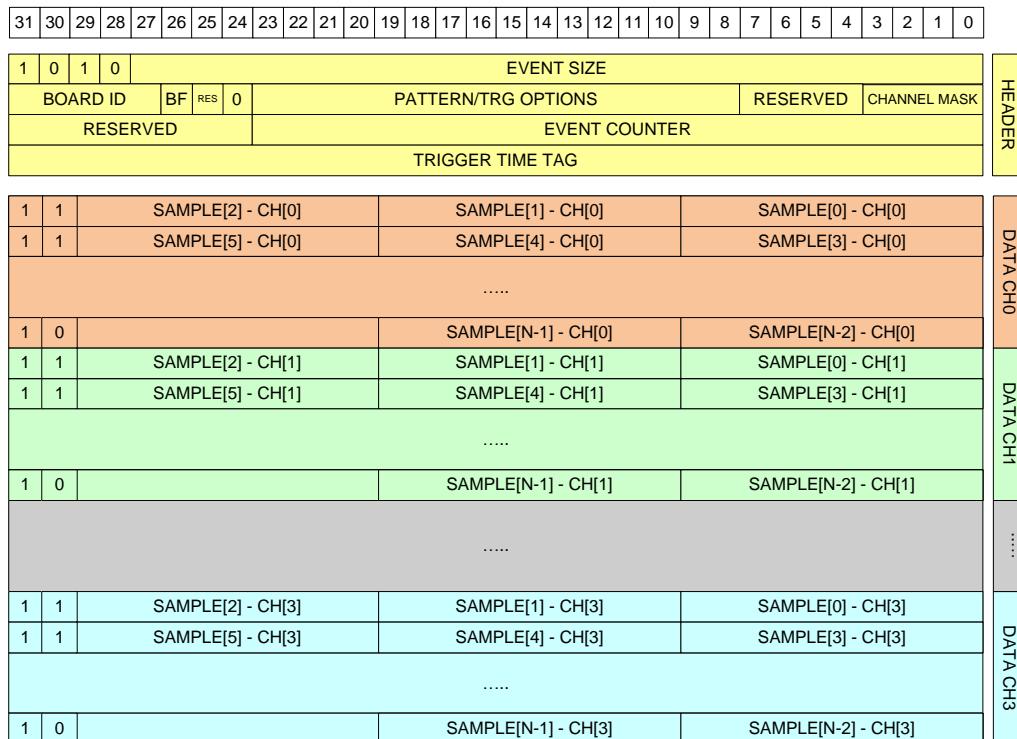


Fig. 9.10: Event Format in Normal Mode.

**Note:** The firmware saves the waveforms in the memory of the digitizer with a granularity of  $n$  (i.e. in groups of  $n$  samples). This way of writing the waveforms in memory allows for a potential  $\Delta T$  between the instant when the trigger physically arrives and when it is sensed by the digitizer. The resulting effect is a jitter in the acquisition window between one event and the next. This jitter can be observed by graphing the waveforms of the enabled channels using an acquisition software. The channels may jitter together between one event and the next, but not among themselves.

### 9.7.6 Acquisition Synchronization

Each channel of the digitizer is provided with a SRAM memory that can be organized in a programmable number  $N_b$  of circular buffers ( $N_b = [1 : 1024]$ , see Tab. 9.1). When the trigger occurs, the FPGA writes

further a programmable number of samples for the post-trigger and freezes the buffer, so that the stored data can be read via USB or Optical Link. The acquisition can continue in a new buffer.

When all buffers are filled, the board is considered FULL: no trigger is accepted and the acquisition stops (i.e. the samples coming from the ADC are not written into the memory, so they are lost). As soon as one buffer is read out and freed, the board exits the FULL condition and acquisition restarts.

**IMPORTANT:** When the acquisition restarts, no trigger is accepted until at least the entire buffer is written. This means that the dead time is extended for a certain time (depending on the size of the acquisition window) after the board exits the FULL condition.

A way to eliminate this extra dead time is by setting bit[5] = 1 at register address 0x8100 **[RD1]**. The board is so programmed to enter the FULL condition when  $N_b - 1$  buffers are filled: no trigger is then accepted, but samples writing continues in the last available buffer. As soon as one buffer is read out and becomes free, the board exits the FULL condition and can immediately accept a new trigger. This way, the FULL reflects the BUSY condition of the board (i.e. inability to accept triggers).



**Note:** when bit[5] = 1, the minimum number of circular buffers to be programmed is  $N_b = 2$ .

In some cases, the BUSY propagation from the digitizer to other parts of the system has some latency and it can happen that one or more triggers occur while the digitizer is already FULL and unable to accept those triggers. This condition causes event loss and it is particularly unsuitable when there are multiple digitizers running synchronously, because the triggers accepted by one board and not by other boards cause event misalignment.

In these cases, it is possible to program the BUSY signal to be asserted when the digitizer is close to FULL condition, but it has still some free buffers (Almost FULL condition). In this mode, the digitizer remains able to accept some more triggers even after the BUSY assertion and the system can tolerate a delay in the inhibit of the trigger generation. When the Almost FULL condition is enabled by setting the Almost FULL level to "X" (register address 0x816C **[RD1]**), the BUSY signal is asserted as soon as X buffers are filled, although the board still goes FULL (and rejects triggers) when the number of filled buffers is  $N_b$  or  $N_b - 1$ , depending on bit[5] at register address 0x8100 as described above.


It is possible to provide the BUSY signal on the digitizer front panel GPO output (bit[20], bits[19:18] and bits[17:16] at register address 0x811C are involved **[RD1]**).

## 9.8 Trigger Management

When operating the waveform recording firmware, all board channels share the same trigger (board common trigger), so they acquire an event simultaneously and in the same way (determined number of samples according to buffer organization and custom size settings, as well as position with respect to the trigger defined by the post-trigger).



**Note:** For the trigger management in the DPP firmware operating, please refer to the DPP documentation [RD2] [RD3].

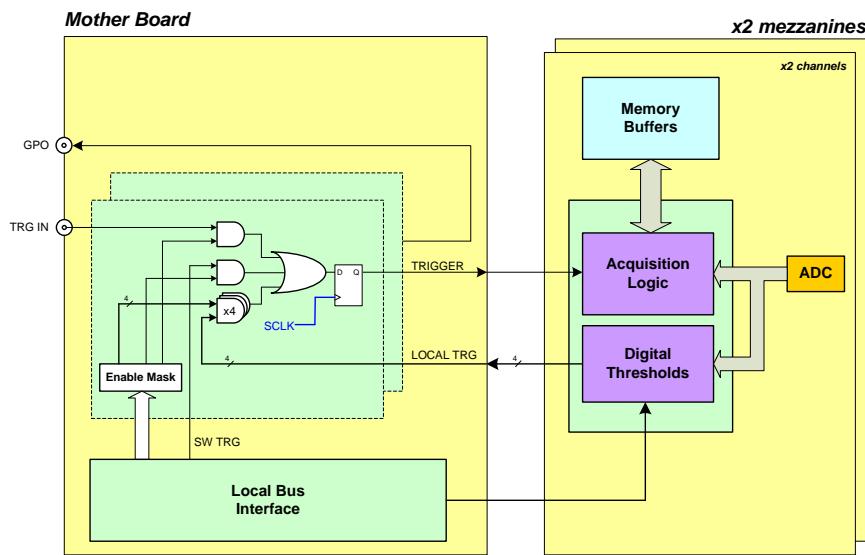

**Fig. 9.11:** Block diagram of Trigger management.

The digitizer supports different sources for the generation of the board common trigger (configurable at register address 0x810C):

- **Software Trigger**
- **External Trigger**
- **Self-trigger**
- **Coincidences**
- **TRG-IN as Gate**

### 9.8.1 Software Trigger

Software triggers are internally produced via software command (write access at register address 0x8108) through USB or Optical Link.

### 9.8.2 External Trigger


A TTL or NIM external signal can be provided to the front panel TRG-IN connector (configurable at register address 0x811C). When setting up a system of multiple digitizers (see Sec. 9.9), there could be a random

jitter of 1 TRG-CLK hit (see Sec. 9.5) if the external signal is provided asynchronously with the internal clock of the boards (e.g. from external trigger FAN-IN on TRG-IN). One board could then sense the trigger at `clock_hit[N]`, while another board at `clock_hit[N+1]` and the same jitter is then present between the pulse acquired by one board and that acquired by the other board.

### 9.8.3 Self-Trigger

Each channel can generate a self-trigger signal (SELF-TRG) when the digitized input pulse exceeds a configurable threshold set through the register address 0x1n80 [RD1].

The individual self-triggers from all channels are propagated to the central trigger logic on the motherboard (see Fig. 9.11) where they participate in logic OR to produce the board common trigger, which is finally distributed back to all channels on the mezzanines causing the event acquisition (see Sec. 9.8.6).

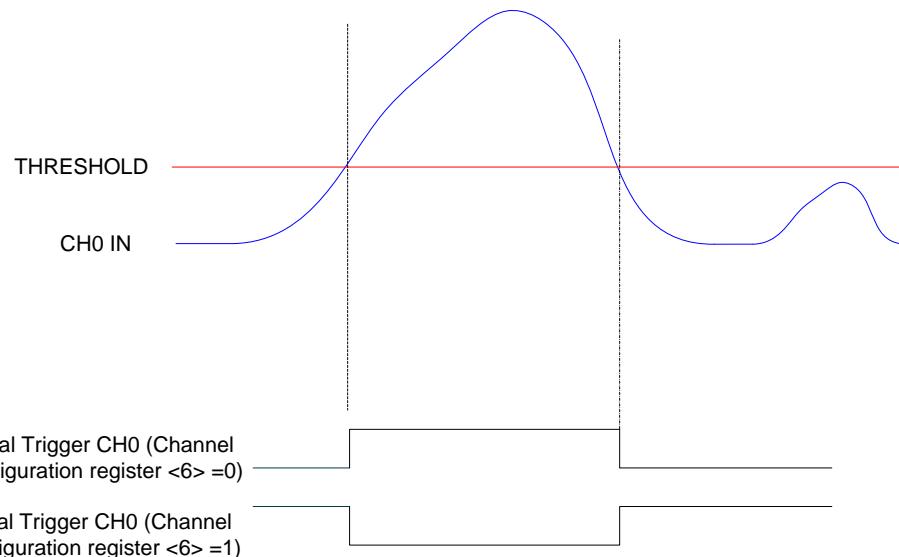

**Fig. 9.12:** Self-trigger generation.

Bits[3:0] of register 0x810C allows the user to program which channel participates to the global trigger generation.

### 9.8.4 Trigger Coincidence Level

Operating the waveform recording firmware, the acquisition trigger is common to the whole board. This common trigger allows the coincidence acquisition mode to be performed through the Majority operation.

Enabling the coincidences is possible by writing at register address 0x810C :

- Bits[3:0] enable a specific channel self-trigger to participate in the coincidence;
- Bits[23:20] set the coincidence window ( $T_{TVAW}$ ) linearly in steps of the Trigger clock (8 ns);
- Bits[26:24] set the Majority (i.e. Coincidence) level;

The coincidence takes place when:

$$\text{Number of enabled channels} > \text{Majority level}$$


Supposing that bits[3:0] = F (i.e. all channels are enabled) and bits[26:24] = 01 (i.e. Majority level = 1), a common trigger is issued whenever at least two of the enabled self-triggers are in coincidence within the programmed  $T_{TVAW}$ .

The Majority level must be smaller than the number of channels enabled via bits[3:0] mask. By default, bits[26:24] = 00 (i.e. Majority level = 0), which means the coincidence acquisition mode is disabled and the  $T_{TVAW}$  is meaningless. In this case, the common trigger is simple OR of the enabled channel self-triggers.




**Note:** in order not to overload the plots but preserve the clearness of concept, only CH0 and CH1 are supposed to be fed with input pulses in the following figures.

**Fig. 9.13** shows the trigger management in case the coincidences are disabled.

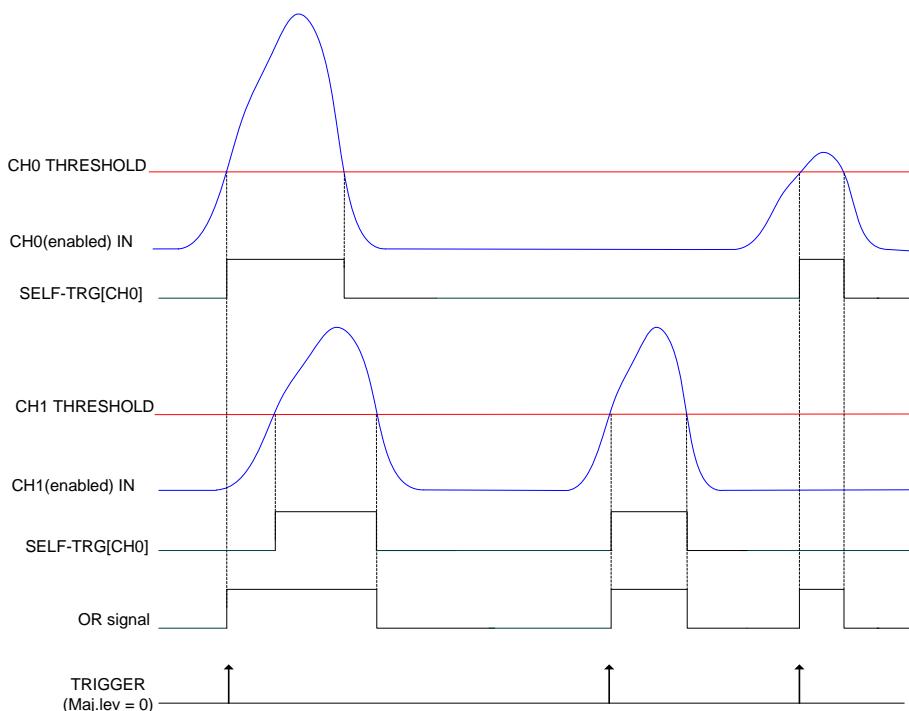

**Fig. 9.13:** Self-trigger relationship with Majority level = 0.

**Fig. 9.14** shows the trigger management in case the coincidences are enabled with Majority level = 1 and  $T_{TVAW}$  is a value different from 0.

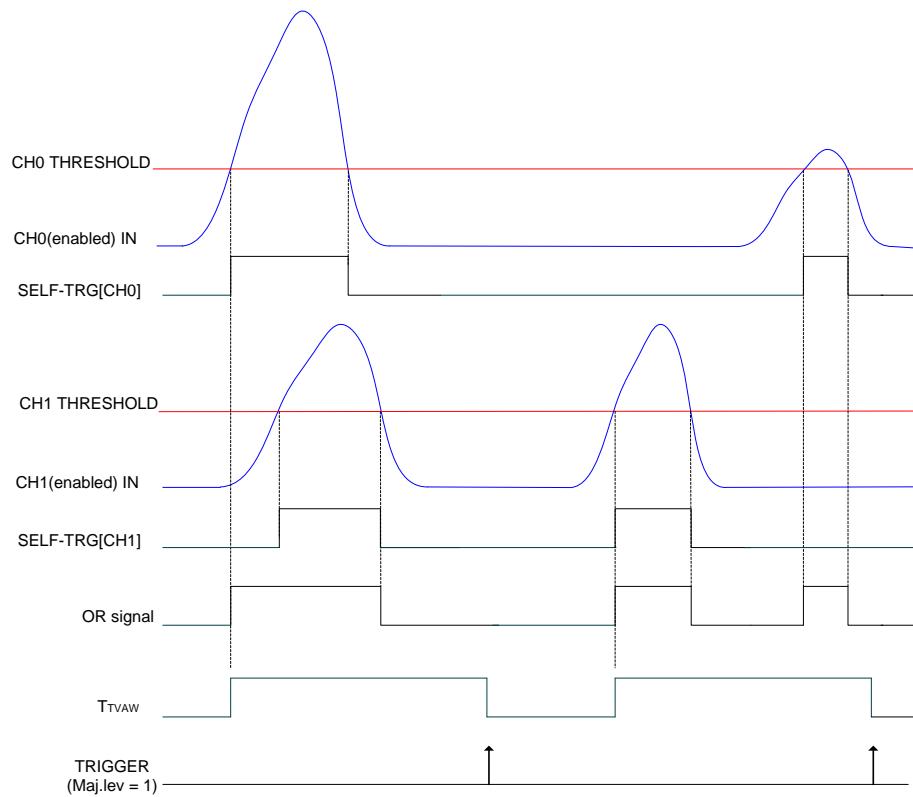

**Fig. 9.14:** Self-trigger relationship with Majority level = 1 and  $T_{TTVAW} \neq 0$ .




**Note:** with respect to the position where the common trigger is generated, the portion of input signal stored depends on the programmed length of the acquisition window and on the post trigger setting.

**Fig. 9.15** shows the trigger management in case the coincidences are enabled with Majority level = 1 and  $T_{TTVAW} = 0$  (i.e. 1 clock cycle).



**Note:** CAEN provides a guide to coincidences including a practical example of making coincidences with the waveform recording firmware **[RD11]**.

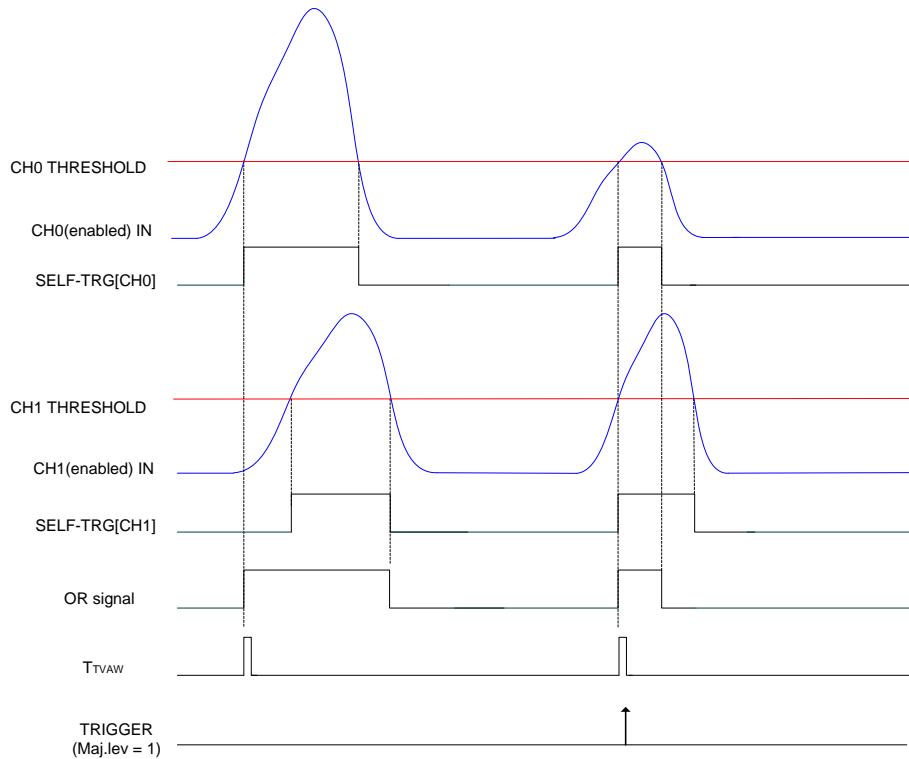

**Fig. 9.15:** Self-trigger relationship with Majority level = 1 and T<sub>TVAW</sub> = 0.

### 9.8.5 TRG-IN as Gate

It is possible to configure TRG-IN as a gate for trigger anti-veto function. The common acquisition trigger is then issued upon the AND between the external signal on TRG-IN and the other trigger sources but the software trigger (i.e. the software trigger cannot participate in the Trigger as Gate mode).

This mode is enabled by setting bit[27] = 1 of register 0x810C and bit[10] = 1 of register 0x811C. The trigger sources participating in AND with TRG-IN are configurable through register 0x810C as well.

### 9.8.6 Trigger distribution

As described in Sec. 9.8, the OR of all the enabled trigger sources, synchronized with the internal clock, becomes the common trigger of the board that is fed in parallel to all channels, consequently causing the capture of an event. By default, only the Software Trigger and the External Trigger participate in the common acquisition trigger (refer to the red path on top of **Fig. 9.16**).


A Trigger Out signal is also generated on the relevant front panel GPO connector (NIM or TTL), and allows to extend the trigger signal to other boards. Thanks to its configurability, GPO can propagate out:

- the OR of all the enabled trigger sources (only the Software Trigger is provided by default, as in the red path of **Fig. 9.16**);
- the OR, AND or MAJORITY exclusively of the channel self-triggers.

The registers involved in the GPO programming are:

- Register address 0x8110;

- Register address 0x811C.

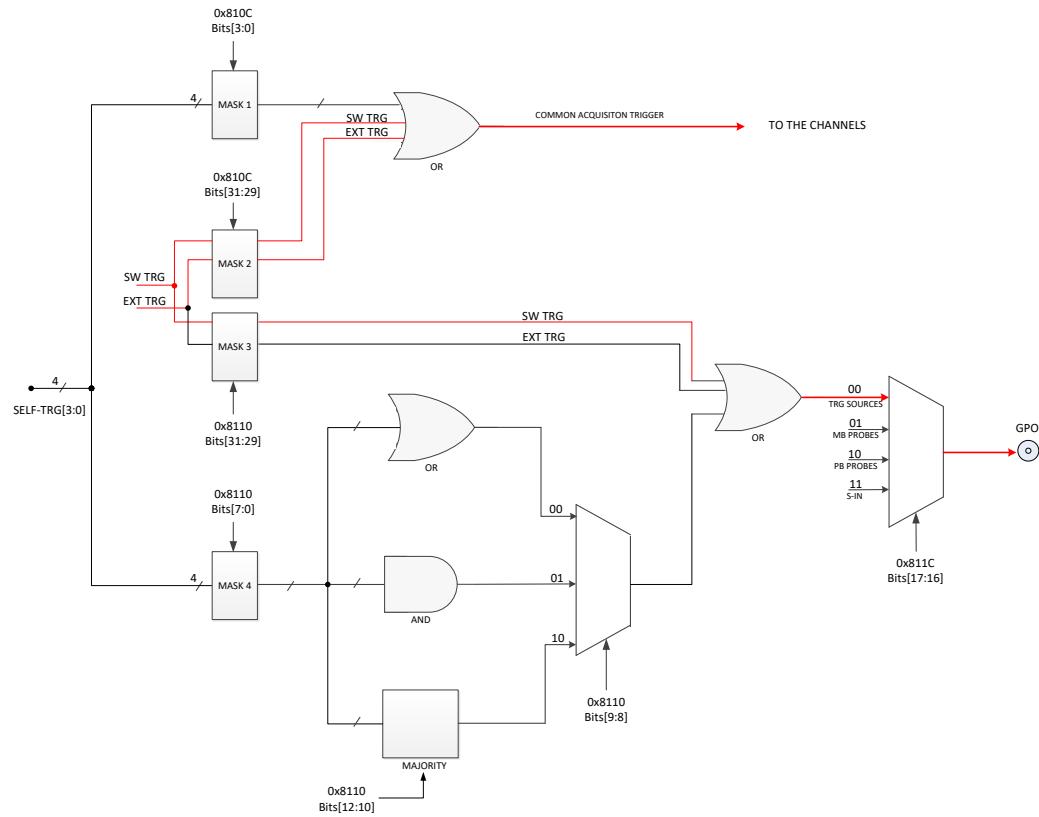

**Fig. 9.16:** Trigger configuration of TRG-OUT front panel connector.

### 9.8.6.1 Example

It could be required to start the acquisition on all the channels of a multi-board system as soon as one of the board channels (board “n”) crosses its threshold. Trigger Out signal is then fed to an external Fan Out logic unit (e.g. CAEN V2495 board); the obtained signal has then to be provided to the external trigger input TRG-IN of all the boards in the system (including the board which generated the Trigger Out signal). In this case, the programming steps to perform are thereafter described.

1. Register 0x8110 on board “n”:
  - Enable the desired self-trigger as Trigger Out signal on board “n” (by bits[3:0] mask).
  - Disable Software Trigger, External Trigger as Trigger Out signal on board “n” (bits[31:30] = 00).
  - Set Trigger Out signal as the OR of the enabled self-trigger on board “n” (bits[9:8] = 00).
2. Register 0x811C on board “n”:
  - Configure the digitizer to propagate on GPO the internal trigger sources according to the 0x8110 settings (i.e. the enabled self-trigger, in the specific case) on board “n” (bits[17:16] = 00).
3. Register 0x810C on all the boards in the system (including board “n”):
  - Enable External Trigger to participate in the board common acquisition trigger, disable Software Trigger and the channel self-triggers (bits[31:30] = 01; bits[3:0] = 0000).


## 9.9 Multi-board Synchronization

When multi-board systems are involved in an experiment, it is necessary to synchronize different boards. In this way, the user can acquire from  $N$  boards with  $Y$  channel each, like if they were just one board with  $(N \times Y)$  channels. While all the channels of the same board are simultaneously sampled at the same clock frequency by design, the main issue with a multi-board system is to guarantee the clock synchronization for the channels of all the boards. This is achieved by using an external clock unit, like CAEN DT4700, which generates the needed reference clock and can provide it in fan-out on the CLK-IN connector of up to ten digitizers.

Other issues are the synchronization of the start of the run to let all the boards have the same zero for time stamps, the trigger synchronization to propagate and combine the triggers from all the boards to have the same common acquisition trigger, and the event data synchronization to keep event data aligned across boards (busy/veto management). For a detailed guide to multi-board synchronization, refer to [\[RD12\]](#), or contact CAEN for clarifications (see Chap. 14).

## 9.10 Test Pattern Generator

The FPGA AMIC can emulate the ADC and write into memory a sawtooth signal for test purposes. It can be enabled via register 0x8000. **Fig. 9.17** shows the test ramps for even and odd channels respectively.

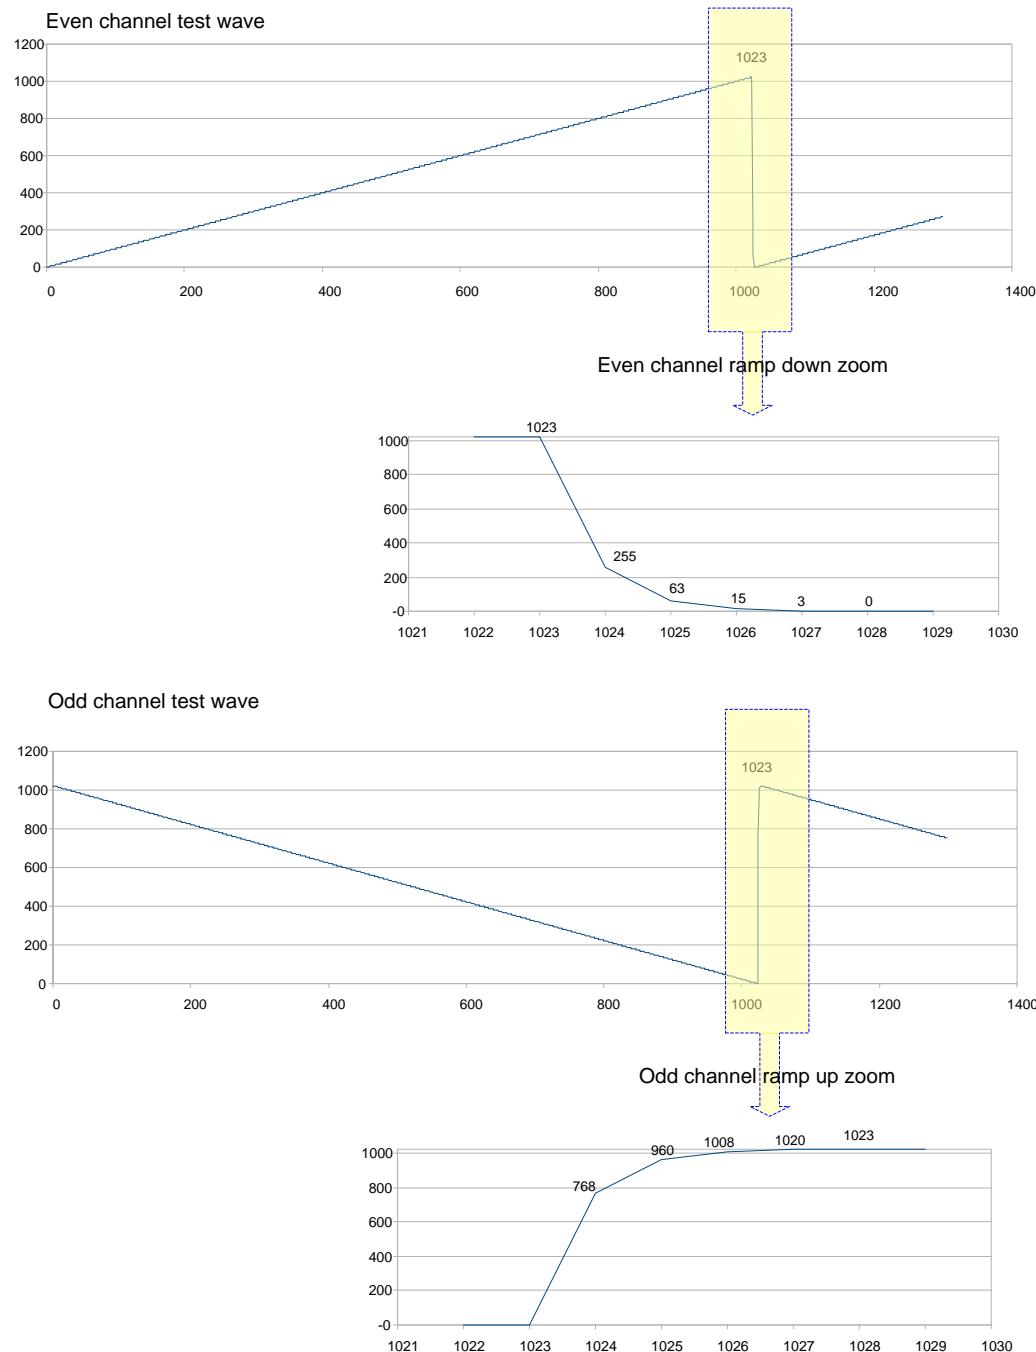

**Fig. 9.17:** FPGA Test Waveform.

## 9.11 Reset, Clear and Default Configuration

### 9.11.1 Global Reset

Global Reset is performed at power-on of the module or via software by write access at register address 0xEF24 . It allows to clear the data off the Output Buffer, the event counter and performs a FPGAs global reset, which restores the FPGAs to the default configuration. It initializes all counters to their initial state and clears all detected error conditions.

### 9.11.2 Memory Reset

The Memory Reset clears the data off the Output Buffer.

The Memory Reset can be forwarded via a write access at register address 0xEF28.

### 9.11.3 Timer Reset

The Timer Reset allows to initialize the timer which tags an event. Time counters are reset after a SW Clear command (register address 0xEF28); the reset (leading edge sensitive) can also be forwarded with a pulse sent to the GPI input (leading edge sensitive).In case the GPI connector needs to be used to reset the trigger time stamps, no configurations or access to registers are necessary. The user only has to transmit a NIM or TTL signal to the input, depending on the software selected logic level for the GPI connector. The time stamps reset occurs at every leading edge of the logic signal sent to the GPI connector.

## 9.12 Data Transfer Capabilities and Events Readout

The board features a Multi-Event digital memory per channel, configurable by the user to be divided into 1 up to 1024 buffers, as detailed in Sec. 9.7.4. Once they are written in the memory, the events become available for readout via USB or Optical Link. During the memory readout, the board can store other events (independently from the readout) on the available free buffers.

The events are read out sequentially and completely, starting from the Header of the first available event, followed by the samples of the enabled channels (from 0 to 3) as reported in Fig. 9.10. Once an event is completed, the relevant memory buffer becomes free and ready to be written again (old data are lost). After the last word in an event, the first word (Header) of the subsequent event is readout. It is not possible to read out an event partially.

The size of an event (EVENT SIZE) is configurable and depends on register addresses 0x8020 and 0x800C, as well as on the number of enabled channels.

### 9.12.1 Block Transfer

The Block Transfer readout mode allows to read N complete events sequentially, where N is set at register address 0xEF1C, or by using the *SetMaxNumEventsBLT* function of the CAENDigitizer library [RD9].

When developing programs, the readout process can be implemented on different basis:

- Using **Interrupts**: as soon as the programmed number of events is available for readout, the board sends an interrupt to the PC over the optical communication link (not supported by USB and A4818).
- Using **Polling** (interrupts disabled): by performing periodic read accesses to a specific register of the board it is possible to know the number of events present in the board and perform a BLT read of the specific size to read them out.
- Using **Continuous Read** (interrupts disabled): continuous data read of the maximum allowed size (e.g. total memory size) is performed by the software without polling the board. The actual size of the block read is determined by the board that terminates the BLT access at the end of the data, according to the configuration of register address 0xEF1C, or the library function *SetMaxNumEventsBLT* mentioned above. If the board is empty, the BLT access is immediately terminated and the “Read Block” function will return 0 bytes (it is the *ReadData* function in the CAENDigitizer Library [RD9]).

Independently from above method, it is suggested to ask the board for the maximum of events per block being set. Furthermore, the greater this maximum, the greater the readout efficiency, despite a larger memory allocation required on the host station this is not a real drawback considering nowadays personal computers.

### 9.12.2 Single Data Transfer

This mode allows the user to readout a word per time, from the header (actually 4 words) of the first available event, followed by all the words until the end of the event, then the second event is transferred. The exact sequence of the transferred words is shown in Sec. 9.7.5.

It is suggested, after the 1st word is transferred, to check the EVENT SIZE information and then do as many cycles as necessary (actually EVENT SIZE -1) in order to read completely the event.

## 9.13 Optical Link and USB Access

The board houses a USB2.0 compliant port, providing a transfer rate up to 30 MB/s, and a daisy chainable Optical Link (communication path which uses optical fiber cables as physical transmission line) able to transfer data at 80 MB/s supported by CAEN A2818 PCI, A3818 PCIe controllers, and A4818 USB3 adapter (see **Tab. 1.1**).

A single link can connect up to 8 digitizers in Daisy chain, so a maximum of 8 boards can be Daisy chained by the single-link A2818 card or the A4818 adapter, and a maximum of 32 boards by the 4-link A3818 card (A3818C).

All the information on CAEN PCI/PCIe controllers and PCIe adapter can be found on CAEN website at the A2818, A3818, and A4818 pages.

The parameters for read/write accesses via optical link are Address Modifier, Base Address, data Width, etc. Wrong parameter settings cause Bus Error.

Bit[3] at register address 0xEF00 enables the module to broadcast an interrupt request on the Optical Link (not supported on A4818); the enabled Optical Link Controllers propagate the interrupt on the PCI bus when a request from the Optical Link is sensed. Interrupts can also be managed at the CAENDigitizer library level **[RD9]**.



**Note:** CONET2 is CAEN proprietary serial protocol developed to allow the optical link communication between the host PC, equipped with a A2818 or a A3818 Controller, or a A4818 Adapter, and a CAEN CONET slave. CONET2 is 50% more efficient in the data rate transfer than the previous CONET1 version. The two protocol versions are not compliant to each other and before to migrate from CONET1 to CONET2 it is recommended to read the instructions provided by CAEN in the dedicated Application Note **[RD13]**.



**Note:** The CONET protocol implemented in the A4818 adapter from USB-3.0 to Optical Link does not support the interrupts.

# 10 Drivers & Libraries

## 10.1 Drivers

In order to interface with the board, CAEN provides the drivers for the supported physical communication channels and compliant with Windows® and Linux® OS:

- **CONET Optical Link**, managed by the A2818 PCI card (Obsolete), the A3818 PCIe card or the A4818 Adapter. The driver installation package is available on CAEN website in the “Software/Firmware” tab at the A2818, A3818 and A4818 pages, respectively (**login required**).



**Note:** For the installation of the Optical Link driver, refer to the controller User Manuals **[RD14]**, **[RD15]** and adapter Data Sheet **[RD16]**.

- **USB 2.0 link**, the driver installation packages are downloadable for free on CAEN website at the digitizer page (**login required**).
- **USB 3.0 link**, managed by the A4818 Adapter. The driver installation packages (Windows users only) are downloadable for free on CAEN website at the A4818 page (**login required**).



**Note:** To install the USB link driver on Windows OS, refer to the dedicated Guide **[RD17]**. Linux users can follow the installation instructions of the ReadMe file included in the packet.

## 10.2 Libraries

CAEN libraries are a set of middleware software required by CAEN software tools for a correct functioning. These libraries, including also demo and example programs, represent a powerful base for users who want to develop customized applications for the digitizer control (communication, configuration, readout, etc.):

- **CAENDigitizer** **[RD9]** is a library of C functions specifically designed for the Digitizer families and supports both waveform recording and DPP firmware. The CAENDigitizer library is based on the CAENComm which, in turn, is based on CAENVMELib. For this reason, **the CAENVMELib and CAENComm libraries must be already installed on the host PC before installing the CAENDigitizer**.
- **CAENComm** library **[RD18]** manages the communication at low level (read and write access). The purpose of this library is to implement a common interface to the higher software layers, masking the details of the physical channel and its protocol, thus making the libraries and applications that rely on the CAENComm independent from the physical layer. **The CAENComm requires the CAENVMELib library (access to the VME bus), even in the cases where the VME is not used.**

Installation packages are available for free download on CAEN web site ([www.caen.it](http://www.caen.it)) at each library page (**login required**).

CAENComm (and other libraries here described) supports the following communication channels (**Fig. 10.1**):

PC → USB → DT5751 Digitizer

PC → USB3 → A4818 → CONET → DT5751 Digitizer


PC → PCI (A2818) → CONET → DT5751 Digitizer

PC → PCIe (A3818) → CONET → DT5751 Digitizer

**WHEN TO INSTALL CAEN LIBRARIES:**

**WINDOWS® and LINUX® compliant customized software.** The user must install the required libraries apart.

**LINUX® compliant non-stand alone CAEN software.** The user must install the required libraries apart to run the software.

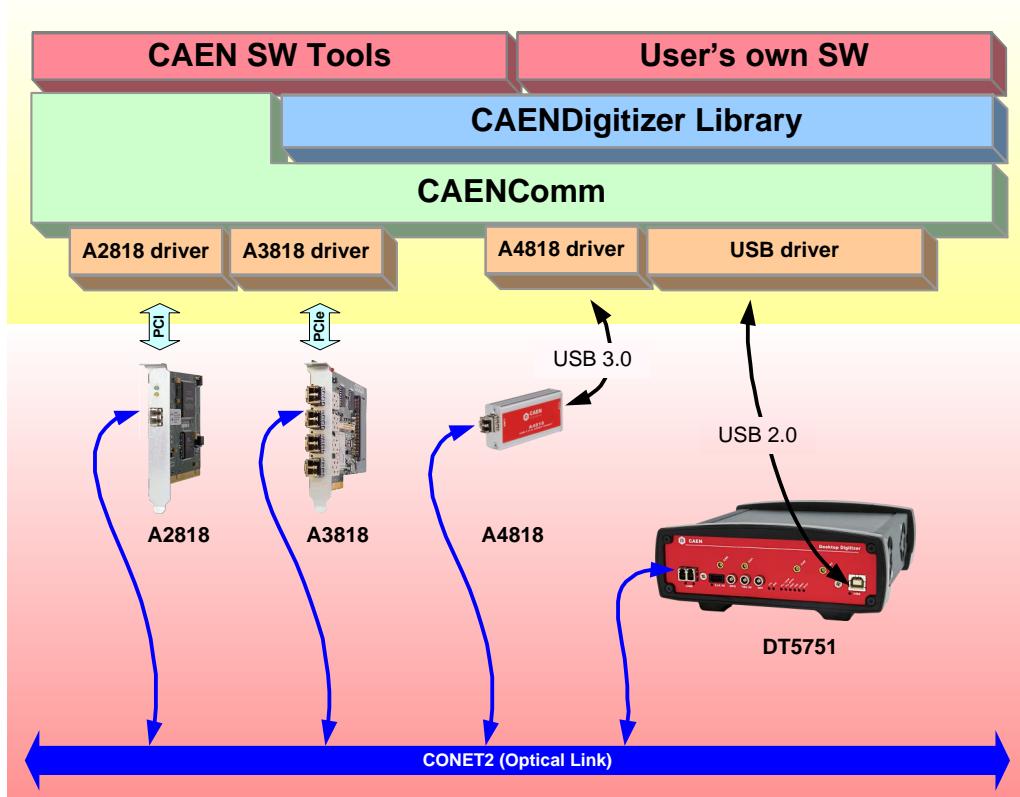

**Fig. 10.1:** Drivers and software layers.

# 11 Software Tools


CAEN provides software tools to interface the 751 digitizer family, which are available for [free download](#) on CAEN web site ([www.caen.it](http://www.caen.it)) in the software and firmware product pages (**login required**).

## 11.1 CAENUpgrader

CAENUpgrader is free software composed of command line tools together with a Java Graphical User Interface.

CAENUpgrader, for the DT5751, allows in few easy steps to:

- Upgrade the FPGA firmware of the board
- Read the FPGA firmware release of the board and the Controller (when included in the communication chain)
- Load a programming file to configure the internal PLL
- Get the Board Info file
- Manage the reboot of the FPGA firmware from the Backup or the Standard FLASH page.

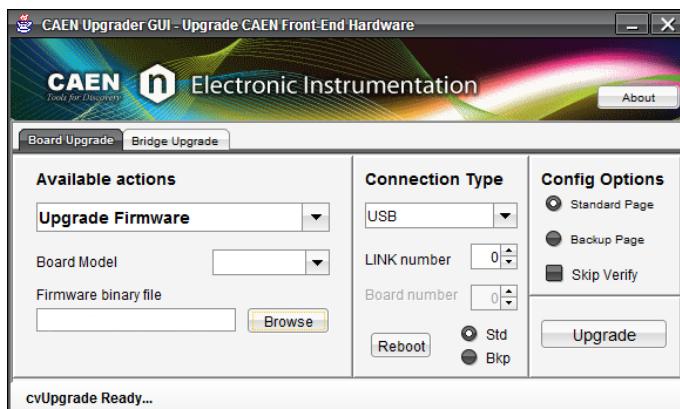

**Fig. 11.1:** CAENUpgrader Graphical User Interface.

CAENUpgrader runs on Windows® and Linux® platforms, 32 and 64-bit operating systems. User must also install the required third-party Oracle Java RE 8 u40 or higher.

The software relies on the CAENComm library (see Chap. 10).


**Note:** CAENUpgrader for Windows® is stand-alone, the user needs to install only the driver for the communication link, while the software locally installs the DLLs of the required libraries.

The Linux® version of the software needs the required CAENVME and CAENComm libraries to be installed apart by the user.

Refer to the CAENUpgrader documentation for installation instructions and for a detailed description [RD5].

## 11.2 CAENComm Demo

CAENComm Demo is simple software developed in C/C++ source code and provided both with Java™ and LabVIEW™ GUI interface. The demo mainly allows for a full board configuration at low level by direct read/write access to the registers and may be used as a debug instrument.

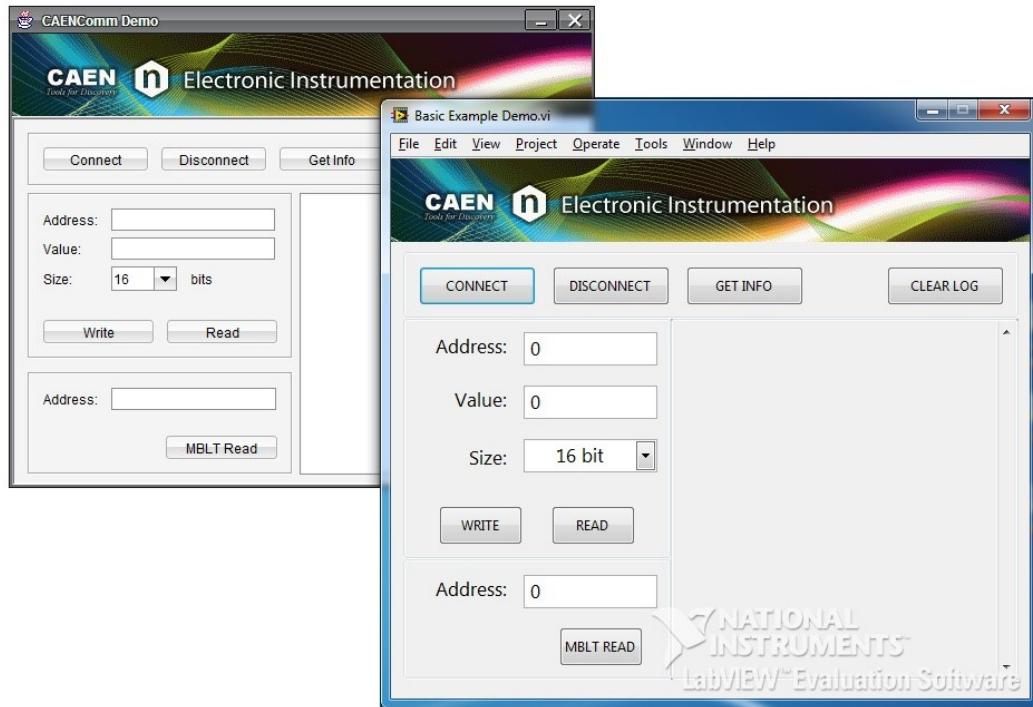

**Fig. 11.2:** CAENComm Demo Java and LabVIEW graphical interface.


The Demo is included in the CAENComm library Windows® installation package only.

Refer to the CAENComm documentation for installation instructions and for a detailed description [RD18].

## 11.3 CAEN WaveDump

WaveDump is a basic console application, with no graphics, supporting only CAEN digitizers running the waveform recording firmware. It allows the user to program a single board (according to a text configuration file containing a list of parameters and instructions), to start/stop the acquisition, read the data, display the readout and trigger rate, apply some post-processing (e.g. FFT and amplitude histogram), save data to a file and also plot the waveforms using Gnuplot third-party graphing utility ([www.gnuplot.info](http://www.gnuplot.info)).

WaveDump is a very helpful example of C code demonstrating the use of libraries and methods for an efficient readout and data analysis. Thanks to the included source files and the VS project, starting with this demo is strongly recommended to all those users willing to write the software on their own.

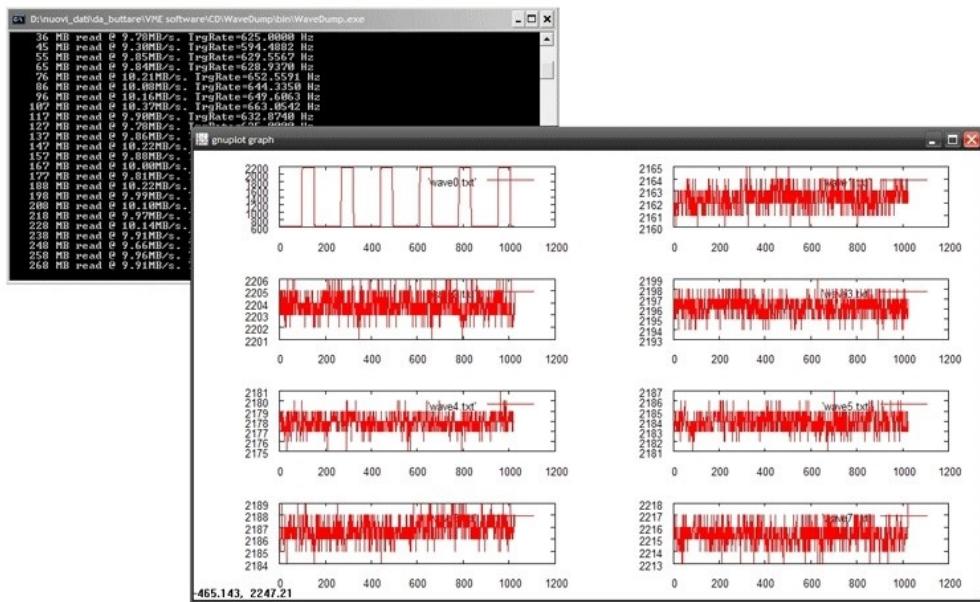

**Fig. 11.3:** CAEN WaveDump.

CAEN WaveDump runs on Windows® and Linux® platforms; Linux users are required to install the third-party Gnuplot.

The software relies on the CAENDigitizer and CAENComm libraries (see Chap. 10).

**Note:** WaveDump for Windows® is stand-alone, the user needs to install only the driver for the communication link, while the software locally installs the DLLs of the required libraries.

The Linux® version of the software needs the required CAENVMElib and CAENComm libraries to be installed apart by the user.

Refer to the WaveDump documentation for installation instructions and for a detailed description [RD10].


CAEN WaveDump does not work with digitizers running DPP firmware.

## 11.4 CoMPASS

CoMPASS (CAEN Multi-PArameter Spectroscopy Software) is the new software from CAEN able to implement a Multi-parametric DAQ for Physics Applications, where the detectors can be connected directly to the digitizers inputs and the software acquires energy, timing, and PSD spectra.

CoMPASS software has been designed as a user-friendly interface to manage the acquisition with all the CAEN DPP algorithm. CoMPASS can manage multiple boards, even in synchronized mode, and the event correlation between different channels (hardware and/or software), apply energy and PSD cuts, calculate and show the statistics (trigger rates, data throughput, etc...), save the output data files (raw data, lists, waveforms, spectra) and use the saved files to run off-line with different processing parameters.

CoMPASS Software supports CAEN first generation digitizers x720, x724, x725, x730, x740D, x751 digitizer families running the DPP-PSD, DPP-PHA and DPP-QDC firmware, the x780, x781 and x782 MCA family, the DT5790 Pulse Processor and the second generation digitizer x2740, x2745 and x2730 running the DPP-PSD and DPP-PHA firmware.

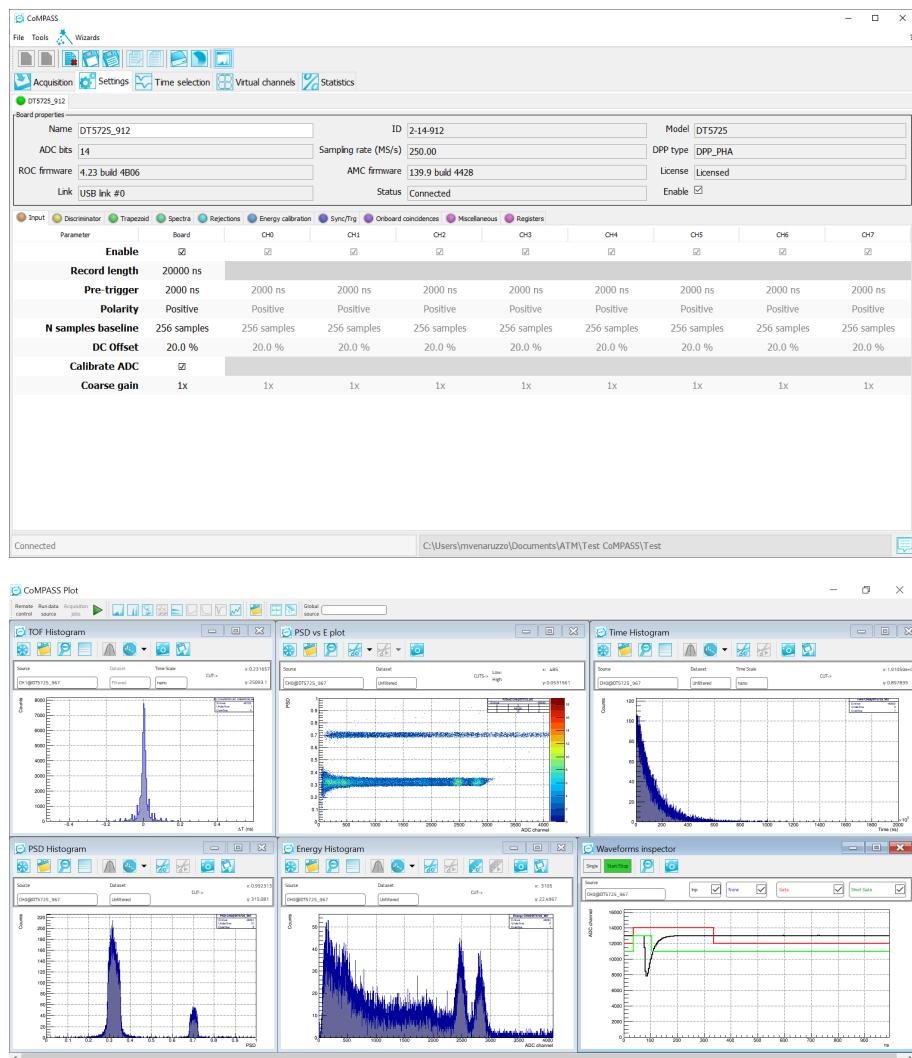

**Fig. 11.4:** CoMPASS software tool.

Refer to CoMPASS documentation for installation instructions and a detailed description [RD2].



CoMPASS does not work with waveform recording firmware.

## 11.5 DPP-ZLE*plus* Control Software

DPP-ZLEplus Control Software is a demo application introducing the user to understand the principle of operation of the Digital Pulse Processing for the Zero Length Encoding (DPP-ZLEplus).

The user can make an entire acquisition through this software, as well use the source code to develop his/her customized readout program. Indeed, the package includes the C source files and the Visual Studio project.

The DPP-ZLE*plus* Control Software is a C-based application that programs the Digitizer according to a set of parameters in the configuration text file, starts/stops the acquisition and manages the data readout. The waveforms elaborated by the DPP-ZLE*plus* algorithm are plotted using gnuplot, an external plotting tool, or saved to output text files.

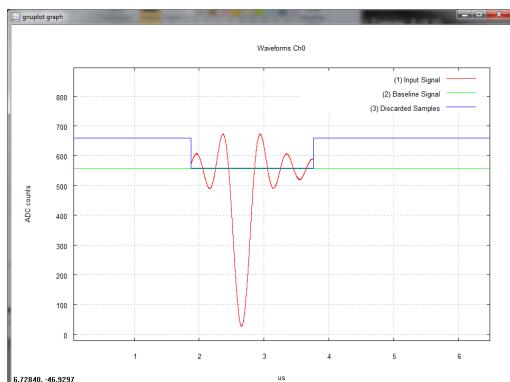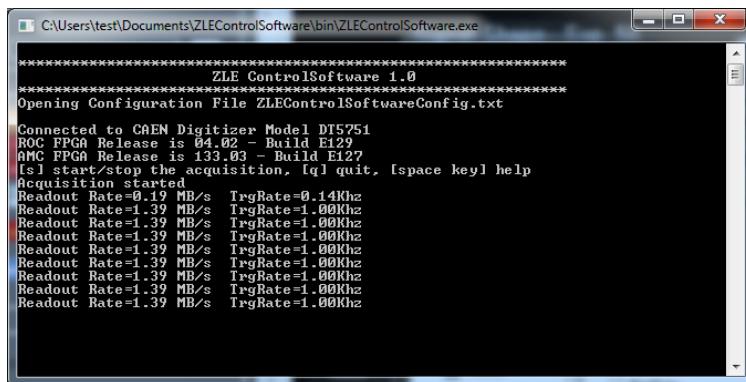

**Fig. 11.5:** Screen-shots of DPP-ZLEplus Control Software.

Refer to the software documentation [RD3] for installation instructions and a detailed.

DPP-ZLEplus Control Software does not work with waveform recording firmware.

## 12 HW Installation

To power on the board, perform the following steps:

1. connect the 12V DC power supply to the DT5751 through the DC input rear connector;
2. power up the DT5751 through the ON/OFF rear switch.



**ONLY QUALIFIED PERSONNEL SHOULD PERFORM INSTALLATION OPERATIONS**



**DO NOT INSTALL THE EQUIPMENT IN A SETUP WHERE IT IS DIFFICULT TO ACCESS THE BACK PANEL FOR DISCONNECTING THE DEVICE**



**IT IS RECOMMENDED THAT THE SWITCH OR CIRCUIT-BREAKER IS NEAR THE EQUIPMENT**



**THE SAFETY OF ANY SYSTEM THAT INCORPORATES THE DEVICE IS UNDER THE RESPONSIBILITY OF THE ASSEMBLER OF THE SYSTEM**

## 12.1 Power-on Status

At power-on, the module is in the following status:

- the Output Buffer is cleared;
- registers are set to their default configuration

After the power-on, only the NIM and PLL LOCK LEDs must stay ON (see **Fig. 12.1**).



**Fig. 12.1:** Front panel LEDs status at power-on.

# 13 Firmware and Upgrades

The board hosts one FPGA on the mainboard and two FPGAs per mezzanine (i.e. one FPGA per channel). The channel FPGAs firmware is identical. A unique file is provided that will update all the FPGAs at the same time.

**ROC FPGA MAINBOARD FPGA (Readout Controller + VME interface):**

FPGA Altera Cyclone EP3C16

**AMC FPGA MEZZANINE FPGA (ADC readout/Memory Controller):**

FPGA Altera Cyclone EP3C16

The firmware is stored onto the on-board FLASH memory. Two copies of the firmware are stored in two different pages of the FLASH, referred to as Standard (STD) and Backup (BKP). In case of waveform recording firmware, the board is delivered equipped with the same firmware version on both pages.

At power-on, a micro-controller reads the FLASH memory and programs the module automatically loading the first working firmware copy, that is the STD one in normal operating.

It is possible to upgrade the board firmware via USB or Optical Link by writing the FLASH with the CAENUpgrader software (see Chap. 11).

**IT IS STRONGLY SUGGESTED TO OPERATE THE DIGITIZER UPON THE STD COPY OF THE FIRMWARE. UPGRADES ARE SO RECOMMENDED ONLY ON THE STD PAGE OF THE FLASH. THE BKP COPY IS TO BE INTENDED ONLY FOR RECOVERY USAGE. IF BOTH PAGES RESULT CORRUPTED, THE USER WILL NO LONGER BE ABLE TO UPLOAD THE FIRMWARE VIA USB OR OPTICAL LINK AGAIN AND THE BOARD NEEDS TO BE SENT TO CAEN FOR REPAIR!**

## 13.1 Firmware Upgrade

Firmware updates are available for download on CAEN website ([www.caen.it](http://www.caen.it)) at the digitizer page (**login required**).

Different firmware are available for the 751 family:

- The waveform recording firmware;
- The special DPP firmware for Physics Applications:
  - DPP-PSD firmware to use the digitizer as a digital replacement Dual Gate QDC, Discriminator and Gate Generator.
  - DPP-ZLEplus firmware to transfer the waveform in a compact format performing an advanced Zero Suppression algorithm.

The waveform recording is free firmware and updates are free downloadable.

 **Note:** The DPP firmware is a paid firmware: the trial version can be free downloaded and is fully functional for a 30-minute per power cycle operation. The user must then purchase a license and store the provided unlock code onto the digitizer to run the firmware and its updates without time limitation. The licence is managed by the CAENUpgrader tool [RD19].



**Note:** The 751 family has been produced with FLASH memory of two different sizes. As a consequence, a DPP firmware compatible with each flash memory size is available. To understand the firmware compatibility, refer to [\[RD20\]](#).

### 13.1.1 Firmware File Description

The programming file is a .CFA (CAEN Firmware Archive) file. It is an archiving file format that aggregates all the programming files of the same firmware kind which are compatible with the same digitizer family.

The name of the CFA file follows a general convention:

- <DIGITIZER>\_rev\_X.Y\_W.Z.CFA for the waveform recording firmware
- <DIGITIZER>\_<DPP\_ALGORITHM>\_rev\_X.Y\_W.Z.CFA for the DPP firmware

where:

- <DIGITIZER> are all the boards that can be updated by the .CFA file. The x751 family includes DT5751, N6751, V1751, VX1751;
- <DPP\_ALGORITHM> is the kind of DPP firmware (options are DPP-PSD, DPP-ZLEplus );
- X.Y is the major/minor revision number of the ROC FPGA;
- W.Z is the major/minor revision number of the AMC FPGA.

To discriminate between the waveform recording firmware and the DPP ones by the firmware version, the reference is the major revision number of the AMC FPGA (W):

- W < 128 means a waveform recording firmware;
- W  $\geq$  128 means a DPP firmware, and it is a fixed number specific for each algorithm and digitizer family. For the 751 series: W=132 means DPP-PSD firmware, W=133 means DPP-ZLEplus firmware.

## 13.2 Troubleshooting

In case of upgrade failure (e.g. STD FLASH page is corrupted), the user can try to reboot the board: after a power cycle, the system programs the board automatically from the alternative FLASH page (e.g. BKP FLASH page), if this is not corrupted as well. The user can so perform a further upgrade attempt on the STD page to restore the firmware copy.



**Note:** old versions of the digitizer motherboard have a slightly different FLASH management. Use CAENUpgrader 1.6.0 or later to get the BoardInfoFile (using the "Get Information" function) and check that the FLASH\_TYPE=0. Alternatively, use a software utility like CAENComm Demo to read at register address 0xF050 and check that bit[7]=0. In this case, at power-on, the micro-controller loads exactly the firmware copy from the STD page of the FLASH .

When a failure occurs during the upgrade of the STD page of the FLASH, which compromises the communication with the DT5751 , the user can perform the following recovering procedure as first attempt:

- force the board to reboot loading the copy of the firmware stored on the BKP page of the FLASH. For this purpose, make sure to connect by USB link and use the Reboot function in CAENUpgrader software by checking "Bkp" option .
- use CAENUpgrader to read the firmware revision (in this case the one of the BKP copy). If this succeeds, it is so possible to communicate again with the board;
- use CAENUpgrader to load the proper firmware file on the STD page, then power-cycle in order the board to get operative again.

If neither of the procedures here described succeeds, it is recommended to send the board back to CAEN in repair (see Chap. [14](#)).

## 14 Technical Support

To contact CAEN specialists for requests on the software, hardware, and board return and repair, it is necessary a MyCAEN+ account on [www.caen.it](http://www.caen.it):


<https://www.caen.it/support-services/getting-started-with-mycaen-portal/>

All the instructions for use the Support platform are in the document:



A paper copy of the document is delivered with CAEN boards.  
The document is downloadable for free in PDF digital format at:

[https://www.caen.it/wp-content/uploads/2022/11/Safety\\_information\\_Product\\_support\\_W.pdf](https://www.caen.it/wp-content/uploads/2022/11/Safety_information_Product_support_W.pdf)

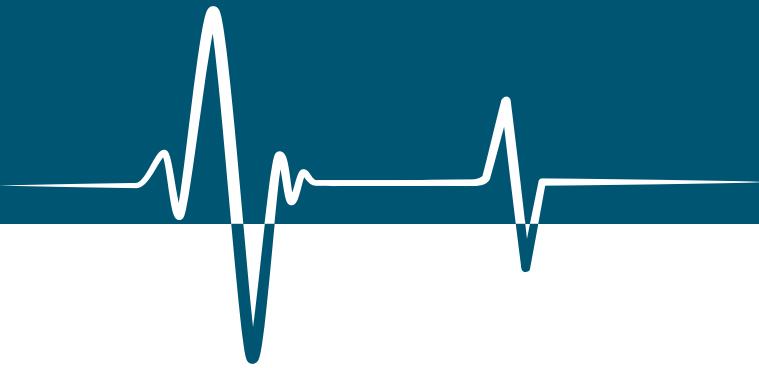**CAEN S.p.A.**

Via Vetraia 11  
55049 - Viareggio  
Italy  
Phone +39 0584 388 398  
Fax +39 0584 388 959  
info@caen.it  
[www.caen.it](http://www.caen.it)

**CAEN GmbH**

Brunnenweg 9  
64331 Weiterstadt  
Germany  
Tel. +49 (0)212 254 4077  
Mobile +49 (0)151 16 548 484  
info@caen-de.com  
[www.caen-de.com](http://www.caen-de.com)

**CAEN Technologies, Inc.**

1 Edgewater Street - Suite 101  
Staten Island, NY 10305  
USA  
Phone: +1 (718) 981-0401  
Fax: +1 (718) 556-9185  
info@caentechnologies.com  
[www.caentechnologies.com](http://www.caentechnologies.com)

**CAENspa INDIA Private Limited**

B205, BLDG42, B Wing,  
Azad Nagar Sangam CHS,  
Mhada Layout, Azad Nagar, Andheri (W)  
Mumbai, Mumbai City,  
Maharashtra, India, 400053  
info@caen-india.in  
[www.caen-india.in](http://www.caen-india.in)



Copyright © CAEN SpA. All rights reserved. Information in this publication supersedes all earlier versions. Specifications subject to change without notice.