



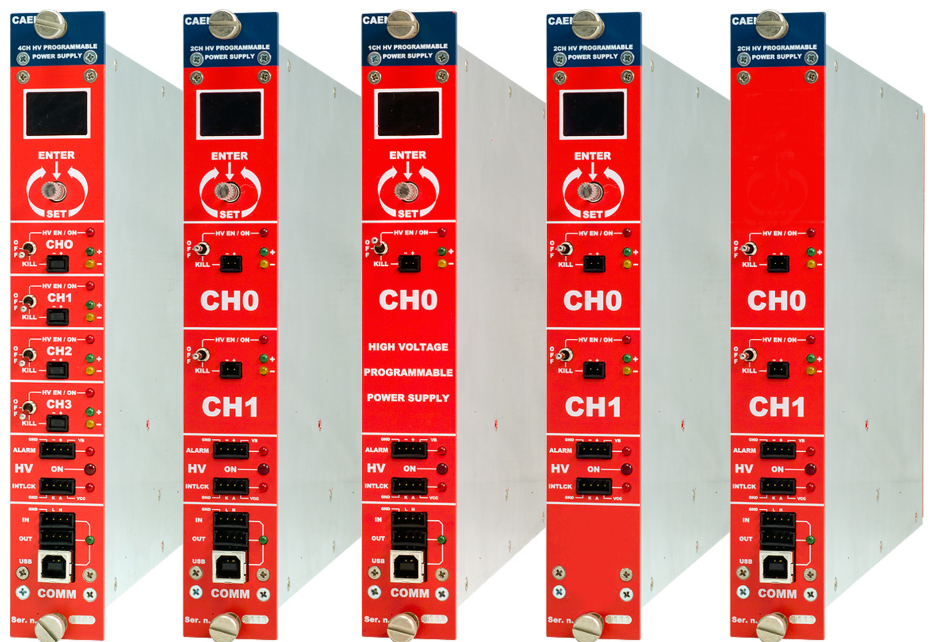

Register your device

Register your device to your **MyCAEN+** account and get access to our customer services, such as notification for new firmware or software upgrade, tracking service procedures or open a ticket for assistance. **MyCAEN+** accounts have a dedicated support service for their registered products. A set of basic information can be shared with the operator, speeding up the troubleshooting process and improving the efficiency of the support interactions.

MyCAEN+ dashboard is designed to offer you a direct access to all our after sales services. Registration is totally free, to create an account go to <https://www.caen.it/become-mycaenplus-user> and fill the registration form with your data.

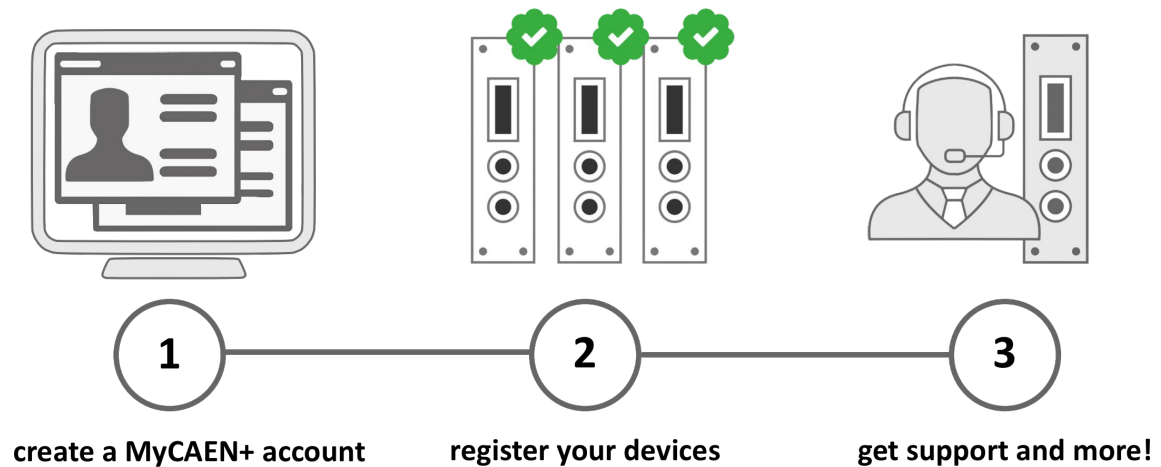

<https://www.caen.it/become-mycaenplus-user/>

Purpose of this Manual

This document is the N1470 User's Manual; it contains information about the installation, the configuration and the use of the unit.

Change Document Record

Date	Revision	Changes
10 July 2017	20	Updated 2.5.1, 3.1, 3.4.1
3 April 2019	21	Updated 2.5.1
31 May 2019	22	Updated 2.7
02 September 2019	23	Updated Table 2.3
11 October 2019	24	Updated IMon Zoom description throughout document
12 February 2021	25	Updated Table 2.3

Symbols, abbreviated terms and notation

T.B.D.

Reference Documents

T.B.D.

Disclaimer

No part of this manual may be reproduced in any form or by any means, electronic, mechanical, recording, or otherwise, without the prior written permission of CAEN SpA.

CAEN will repair or replace any product within the guarantee period if the Guarantor declares that the product is defective due to workmanship or materials and has not been caused by mishandling, negligence on behalf of the User, accident or any abnormal conditions or operations.

CAEN declines all responsibility for damages or injuries caused by an improper use of the Modules due to negligence on behalf of the User. It is strongly recommended to read thoroughly the CAEN User's Manual before any kind of operation. *CAEN reserves the right to change partially or entirely the contents of this Manual at any time and without giving any notice.*

Disposal of the Product *The product must never be dumped in the Municipal Waste. Please check your local regulations for disposal of electronics products.*

Made In Italy : We stress the fact that all the boards are made in Italy because in this globalized world, where getting the lowest possible price for products sometimes translates into poor pay and working conditions for the people who make them, at least you know that who made your board was reasonably paid and worked in a safe environment. (this obviously applies only to the boards marked "Made in Italy", we cannot attest to the manufacturing process of "third party" boards).

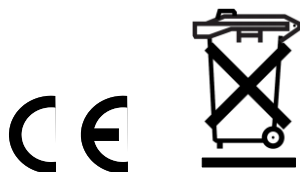


TABLE OF CONTENTS

1	General description.....	6
1.1	Overview	6
2	Technical specifications.....	7
2.1	Packaging.....	7
2.2	Power requirements	7
2.3	Front and back panel	9
2.4	Front panel connections.....	11
2.4.1	Local control section	11
2.4.2	Channel control section	11
2.4.3	HV Status control section	12
2.4.3.1	Alarm signal.....	12
2.4.3.2	Interlock signal.....	12
2.4.4	Remote communication control section.....	13
2.5	Rear panel connections	14
2.5.1	HV Channel Output.....	14
2.6	Imon Zoom	14
2.7	Technical specifications table	15
3	Operating modes.....	16
3.1	Safety requirements and Initial inspection	16
3.2	Programmable parameters	16
3.2.1	Boards parameters	16
3.2.2	Channel settings.....	18
3.3	Local Control	18
3.3.1	HV connection.....	19
3.3.2	Module settings.....	20
3.3.3	Channel settings.....	21
3.3.3.1	Group Settings.....	24
3.3.3.2	Smileys	26
3.4	Remote Control	27
3.4.1	Serial Links	27
3.4.1.1	USB communication	27
3.4.1.2	RS232 communication	28
3.4.1.3	RS485 communication	28
3.4.1.4	Ethernet communication.....	29
3.4.2	Communication Control	30
3.4.2.1	Remote Control: Main Menu	30
3.4.2.2	Remote Control: General Menu	30
3.4.2.3	Remote Control: Channels Menu	30
3.4.2.4	Remote Control: firmware upgrade	31
3.4.2.5	Remote Control: format EEPROM	32
3.5	USB - RS485 Communication Protocol	32
3.5.1	Command Format.....	32
3.5.2	Format of response string.....	33
3.5.3	MONITOR commands related to the Channels.....	33
3.5.3.1	Meaning of STATUS bits (value read in decimal Format).....	34
3.5.4	MONITOR commands related to the module	34
3.5.4.1	Meaning of Board Alarm bits	35
3.5.5	SET commands related to the Channels.....	35
3.5.6	SET commands related to the module	35
4	Internal Settings	36
4.1	Polarity selection	36
4.2	Internal switches	38
4.2.1	Local Bus termination	38
4.2.2	RS485 – RS232 conversion	38
4.3	Grounding specifications.....	38
4.3.1	Safety Earth connection.....	39

LIST OF FIGURES

Fig. 1.1: Mod. Programmable HV Power Supply	6
Fig. 2.1: Backplane NIM connector	8
Fig. 2.2: Mod. N1470 series front panel	9
Fig. 2.3: Mod. N1470 series back panel (std., A, B).....	10
Fig. 2.4: Local control panel	11
Fig. 2.5: Channel control panel and Kill scheme	11
Fig. 2.6: N1470 HV Status control panel	12
Fig. 2.7: N1470 ALARM electrical scheme.....	12
Fig. 2.8: N1470 ALARM TTL configured	12
Fig. 2.9: N1470 INTERLOCK electrical scheme	12
Fig. 2.10: Remote communication control and RS485 I/O – RS232 IN electrical scheme	13
Fig. 2.11: HV Channel panel and test point electrical scheme.....	14
Fig. 3.1: Welcome screen.....	18
Fig. 3.2: Channel OFF status screen	19
Fig. 3.3: Channel ON status screen	19
Fig. 3.4: Channel KILL status screen	19
Fig. 3.5: Mode settings status screen.....	20
Fig. 3.6: Mode settings access screen	20
Fig. 3.7: Mode settings edit screen	20
Fig. 3.8: Channel settings edit screen	21
Fig. 3.9: Channel VSET select screen	21
Fig. 3.10: Channel VSET access screen.....	21
Fig. 3.11: Channel VSET digit selection screen.....	21
Fig. 3.12: Channel VSET digit access screen	22
Fig. 3.13: Channel VSET digit adjust screen.....	22
Fig. 3.14: Channel VSET digit confirm screen	22
Fig. 3.15: Channel VSET confirm screen	22
Fig. 3.16: Channel VSET de-select screen	23
Fig. 3.17: Channel KILL screen	23
Fig. 3.18: Channel EXIT screen	23
Fig. 3.19: Group selection	24
Fig. 3.20: Group active	24
Fig. 3.21: Group VSET access screen	24
Fig. 3.22: Group VSET digit selection screen	24
Fig. 3.23: Group Channel VSET digit access screen.....	25
Fig. 3.24: Group VSET digit adjust screen	25
Fig. 3.25: Group VSET digit confirm screen.....	25
Fig. 3.26: Channel VSET de-select screen	25
Fig. 3.27: Group EXIT screen.....	26
Fig. 3.28: USB communication diagram.....	27
Fig. 3.29: RS232 communication diagram	28
Fig. 3.30: RS485 communication diagram	28
Fig. 3.31: Ethernet communication diagram.....	29
Fig. 3.32: RS232 port cable adapter	29
Fig. 3.33: Main Menu.....	30
Fig. 3.34: Board Status Menu.....	30
Fig. 3.35: Channels Menu	31
Fig. 3.36: PC keyboard.....	31
Fig. 3.37: Channels group setting	31
Fig. 3.38: Firmware Upgrade Menu/1.....	32
Fig. 3.39: Firmware Upgrade Menu/2.....	32
Fig. 3.40: Format EEPROM Menu	32
Fig. 4.1: Side cover removal instructions	36
Fig. 4.2: Polarity selection instructions	37
Fig. 4.3: Dip switch position.....	38
Fig. 4.4: C21 jumper location.....	39
Fig. 4.5: Earth configuration connection examples	40

LIST OF TABLES

Table 1.1: Available items	6
Table 2.1: Power absorption.....	7
Table 2.2: Interlock operation	13
Table 2.3: Mod. N1470 series channel technical specifications.....	15
Table 3.1: Smileys list.....	26

1 General description

1.1 Overview



Fig. 1.1: Mod. Programmable HV Power Supply

The Mod. N1470 provides 4 independent High Voltage channels in a single width NIM mechanics. Two and one channel versions (N1470A and N1470B) are also available. Each channel can provide a $\pm 8\text{kV}$ max voltage, a 3 mA max current and a 9 W max power (8 W max power when output voltage is larger than $\pm 3\text{ kV}$).

Channels have common floating return (common return insulated from the crate ground); HV outputs are delivered through SHV connectors.

The HV output RAMP-UP and RAMP-DOWN rates may be selected independently for each channel in the range $1\div 500\text{ V/s}$ in 1 V/s steps.

Safety features include:

- OVERVOLTAGE and UNDERVOLTAGE warning when the output voltage differs from the programmed value by more than 2% of set value (minimum 10V).
- Programmable VMAX protection limit
- OVERCURRENT detection: if a channel tries to draw a current larger than its programmed limit, it enters TRIP status, keeping the maximum allowed value for a programmable time (TRIP), before being switched off
- Channels can be enabled or disabled individually through the Interlock logic.

Module control can take place either locally, assisted by a Graphic color display (not available on Mod.N1470AR) or remotely, via USB, RS232 or RS485 (not available on Mod.N1470AL); the RS485 port allows to build a N1470s' daisy chain network (up to 32 modules).

For remote operation, CAEN also provides GECO2020, a graphical application that allows to manage the N14xx HV Power Supplies (as well as all other CAEN Power Supplies).

Moreover, these units can be managed via CAEN HV Wrapper, a set of ANSI C functions bundled in a library, providing the software developer an unified software interface for the control of CAEN Power Supplies. This is a low level application in which the writing of the Control SW is assigned to the user. CAEN HV Wrapper is logically located between an higher level application, such as GECO2020, and the lower layer software libraries. It contains a generic software interface independent by the Power Supply models and by the communication path used to exchange data with them. For more info please visit: www.caen.it (products>firmware/software section).

The Mod. A1480 is an optional DC Input Power Equalizer which allows to use a different input power distribution on the N147x modules (see § 2.2).

Table 1.1: Available items

Code	Item	Description
WN1470B08AAC	N1470B	1Ch Programmable Power Supply 8kV
WN1470A08AAC	N1470A	2Ch Programmable Power Supply 8kV
WN1470ALCLAC	N1470AL	2Ch Programmable Power Supply 8kV Local Control (LOW COST)
WN1470ALCRAC	N1470AR	2Ch Programmable Power Supply 8kV Remote Control (LOW COST)
WN1470X08AAC	N1470	4Ch Programmable Power Supply 8kV
WA1480XAAAAA	A1480	DC Power Input Equalizer for N147X Family

2 Technical specifications

2.1 Packaging

The Mod. N1470 boards are housed in single width NIM modules.

2.2 Power requirements

The following table resumes the power absorption in the 3kV/3mA, 4kV/2mA and 8kV/1mA ranges.

Table 2.1: Power absorption


Board type	N1470					
Channel configuration	without A1480			with A1480		
	Max n° CH ON ¹	Current (±12V)	Current (±6V)	Max n° CH ON	Current (±6V)	Current (±12V)
3kV/3mA	3 CH	2.80 A	<10mA	4 CH	4.30 A	1.85 A
4kV/2mA	4 CH	2.84 A	<10mA	4 CH	3.50 A	1.52 A
8kV/1mA	4 CH	3.16 A	<10mA	4 CH	3.90 A	1.68 A
Board type	N1470A, AL, AR					
Channel configuration	without A1480			with A1480		
	Max n° CH ON	Current (±12V)	Current (±6V)	Max n° CH ON	Current (±6V)	Current (±12V)
3kV/3mA	2 CH	1.92 A	<10mA	2 CH	2.32 A	1.04 A
4kV/2mA	2 CH	1.54 A	<10mA	2 CH	1.86 A	0.86 A
8kV/1mA	2 CH	1.58 A	<10mA	2 CH	1.90 A	0.85 A
Board type	N1470B					
Channel configuration	without A1480			with A1480		
	Max n° CH ON	Current (±12V)	Current (±6V)	Max n° CH ON	Current (±6V)	Current (±12V)
3kV/3mA	1 CH	1.09 A	<10mA	1 CH	1.28 A	0.62 A
4kV/2mA	1 CH	0.89 A	<10mA	1 CH	1.05 A	0.52 A
8kV/1mA	1 CH	0.98 A	<10mA	1 CH	1.17 A	0.57 A

WARNING: if the A1480 is not installed, ±6V power supplies are required only by older versions of the N1470; such boards can be recognized by the presence of power pins 10 and 11 on the backplane NIM connector (see figure 2.1). If the A1480 is not installed, new versions operate only with ±12V power supplies.

¹ The maximum number is considered with channels at FULL LOAD

Fig. 2.1: Backplane NIM connector

PIN	FUNCTION
1	+3 Volts
2	-3 Volts
3	SPARE
4	RESERVED
5	COAXIAL
6	COAXIAL
7	COAXIAL
8	+200 Volts D.C.
9	SPARE
10	+6 Volts
11	-6 Volts
12	RESERVED
13	CARRY NO. 1
14	SPARE
15	RESERVED
16	+12 Volts
17	-12 Volts
18	SPARE
19	RESERVED
20	SPARE
21	SPARE
22	RESERVED
23	RESERVED
24	RESERVED
25	RESERVED
26	SPARE
27	SPARE
28	+24 Volts
29	-24 Volts
30	SPARE
31	CARRY NO. 2
32	SPARE
33	117 V A.C. (HOT)
34	POWER RET. GND
35	RESET
36	GATE
37	SPARE
38	COAXIAL
39	COAXIAL
40	COAXIAL
41	117 V A.C. (NEUT.)
42	HIGH QUAL. GND
G	GROUND GUIDE PIN

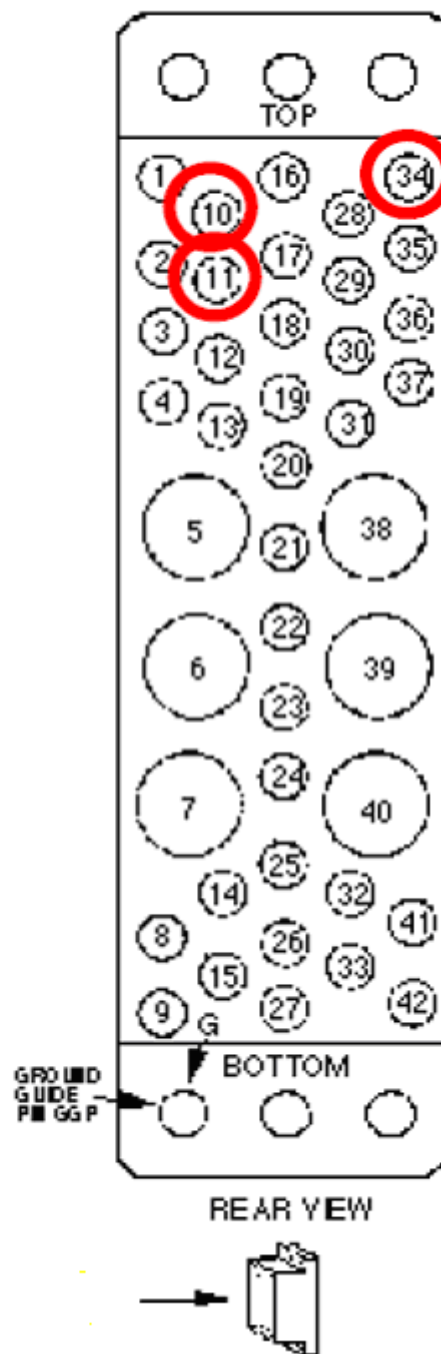

2.3 Front and back panel

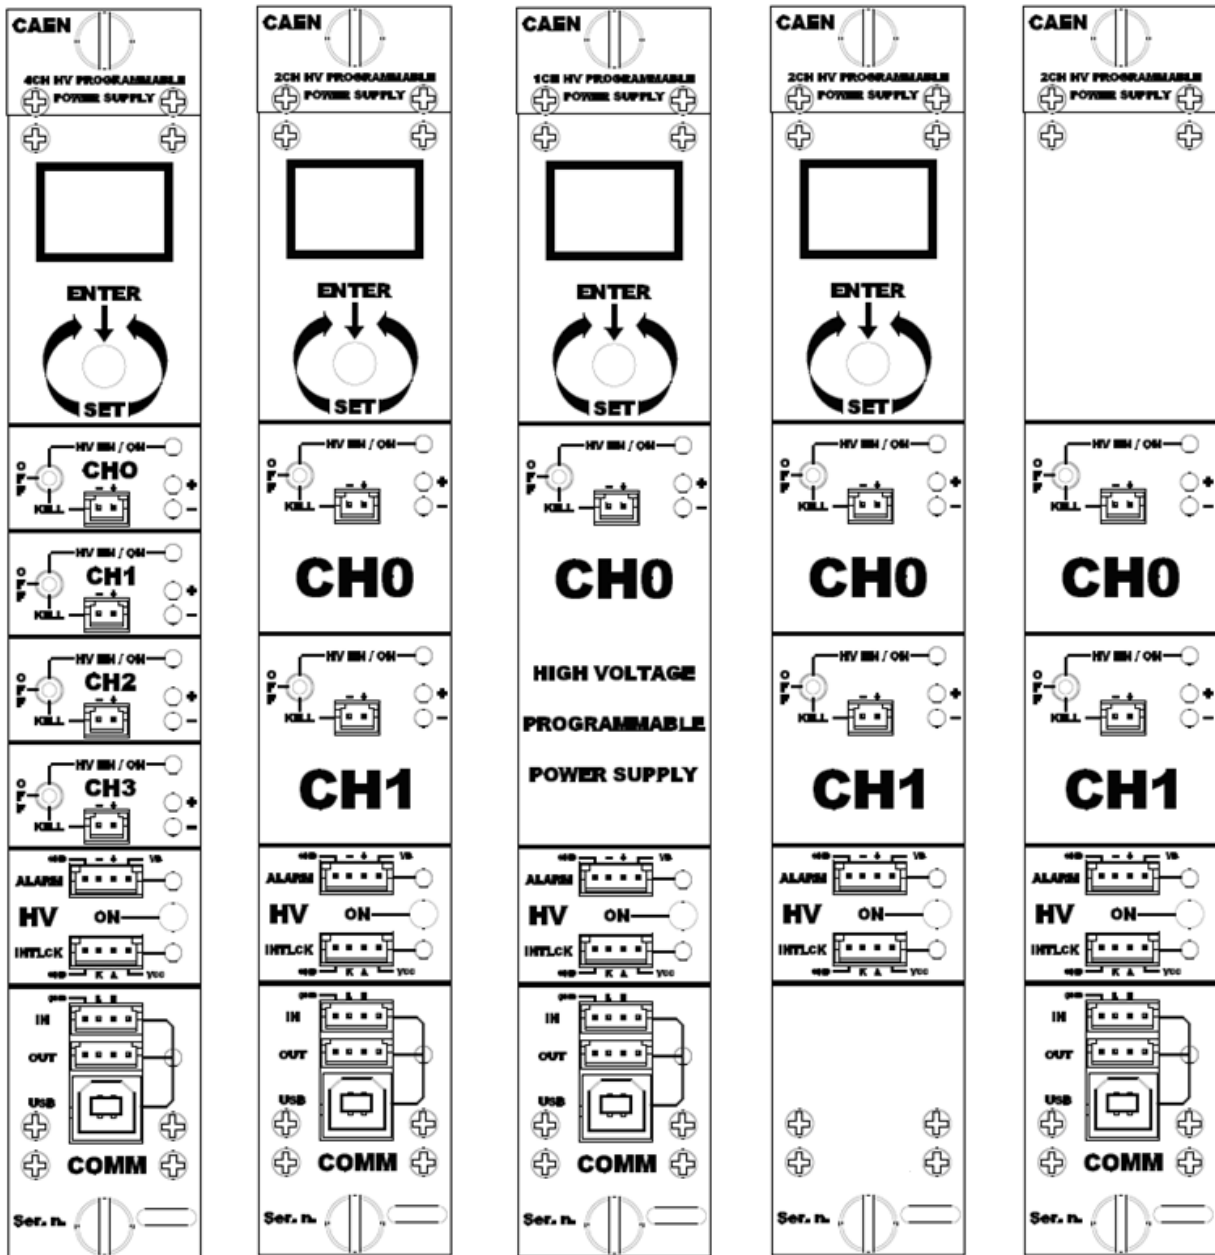


Fig. 2.2: Mod. N1470 series front panel

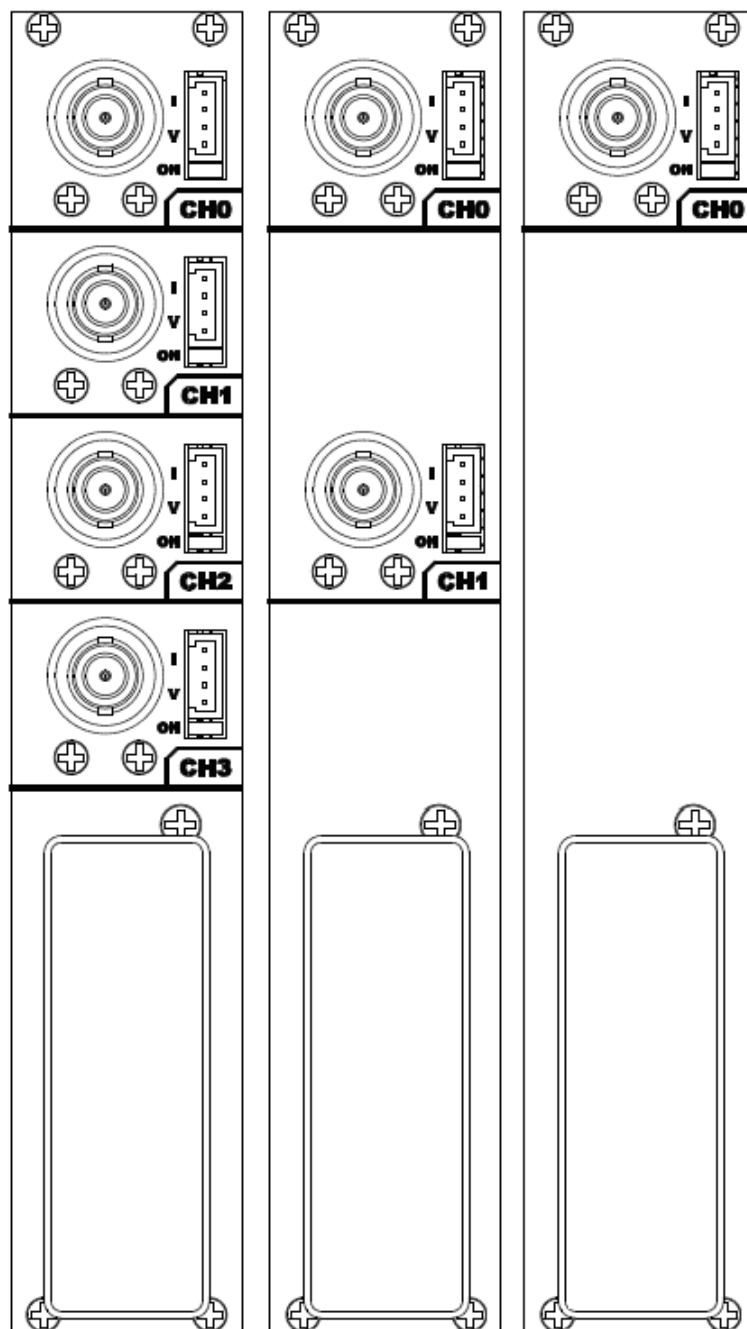


Fig. 2.3: Mod. N1470 series back panel (std., A, B)

2.4 Front panel connections

2.4.1 Local control section²

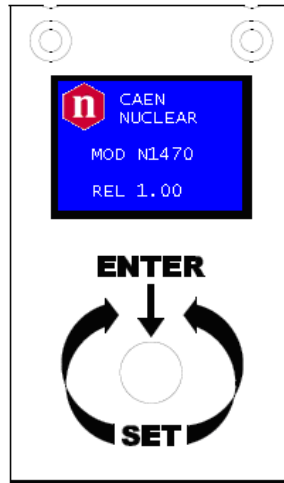


Fig. 2.4: Local control panel

NAME:	TYPE:	FUNCTION:
MONITOR	1" OLED DISPLAY (96x64)	Local settings monitoring
TUNE	ROTARY SWITCH	Parameter and Mode setting

2.4.2 Channel control section

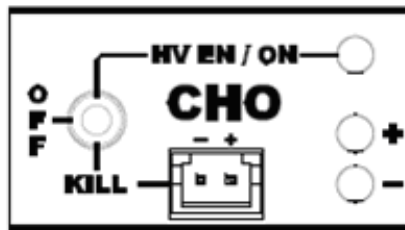


Fig. 2.5: Channel control panel and Kill scheme

NAME:	TYPE:	FUNCTION:
HV_EN/OFF/KILL	3 POS. SWITCH	Channel Enable and turning OFF/KILL ³
ON	RED LED	HV On enabled
REMOTE KILL	AMP 280370-2	The channel is KILLED either as the +/- contacts are open or as a +4÷6Vdc voltage is fed to pin - (see note)
+	GREEN LED	Positive polarity
-	YELLOW LED	Negative polarity

² Not available on Mod. N1470AR

³ OFF: Channel turned off according to RAMP DOWN setting; KILL: Channel turned off at fastest available rate

2.4.3 HV Status control section




Fig. 2.6: N1470 HV Status control panel

NAME:	TYPE:	SIGNAL:	FUNCTION:
ON	RED LED		HV On enabled (at least one channel ON)
ALARM	RED LED/ AMP 280371-2.	Out	Alarm status signaled (active LOW)
INTERLOCK	RED LED/ AMP 280371-2	In	Interlock signal

2.4.3.1 Alarm signal

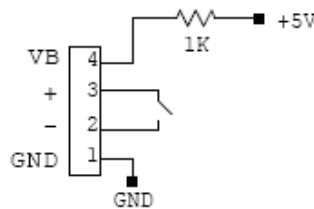


Fig. 2.7: N1470 ALARM electrical scheme

As an Alarm condition is detected (see § 3.5.3.1 and § 3.5.4.1) pins 2 and 3 (- and +) are closed; the contact can be used to switch an external device supplied by an external source, otherwise the VB and GND references can be used to provide a TTL compatible level on pin 2 and 3.

In the first case (externally supplied device) the maximum allowed ratings are:

- Maximum voltage between + and -: 12V
- Maximum sink current across + and -: 100mA

In the latter case, in order to produce a TTL compatible Alarm Out, pin 3 (+) must be connected with pin 4 (VB) and pin 1 (GND) with pin 2 (-); see the diagram below:

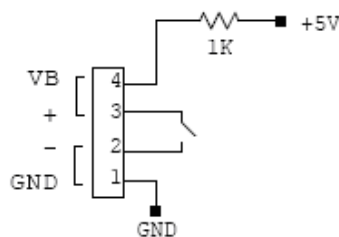


Fig. 2.8: N1470 ALARM TTL configured

2.4.3.2 Interlock signal

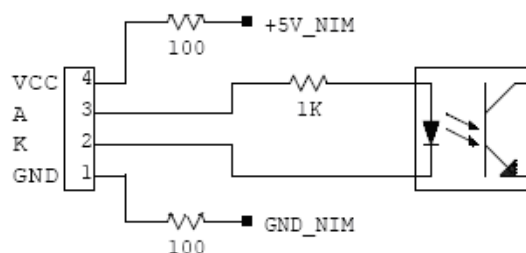


Fig. 2.9: N1470 INTERLOCK electrical scheme

A schematic diagram of the Interlock input is shown in the figure above, where the diode is part of optocoupler stage.

Interlock means that channels are hardware disabled. The interlock operation is explained by the following table:

Table 2.2: Interlock operation

CONFIGURATION ↓	INTERLOCK MODE (§ 3.2.1) →	OPEN	CLOSE
leave contact open		INTERLOCK	ENABLED
voltage level (0÷1V, ~5mA current) between pin 2 and pin 3		INTERLOCK	ENABLED
short circuit pin 1 with pin 2, and pin 3 with pin 4		ENABLED	INTERLOCK
voltage level (4÷6V, ~5mA current) between pin 2 and pin 3		ENABLED	INTERLOCK

The front panel Interlock LED is ON when the INTERLOCK is enabled; as INTERLOCK is enabled, channels are turned off at the fastest available rate, regardless the RAMP DOWN setting.

2.4.4 Remote communication control section⁴

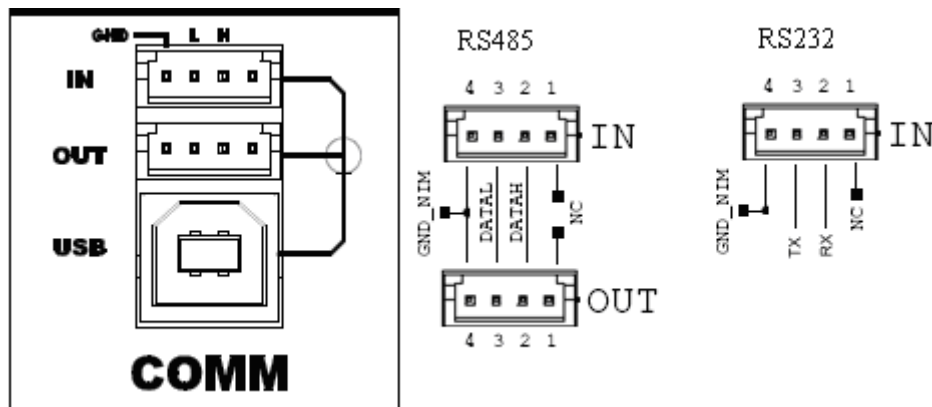


Fig. 2.10: Remote communication control and RS485 I/O – RS232 IN electrical scheme

NAME:	TYPE:	FUNCTION:
IN	AMP 280371-2	RS485 Input ⁵ ; adaptable to RS232 standard (see also § 4.2.2)
OUT	AMP 280371-2	RS485 Output
USB	B TYPE USB	USB2.0 compliant realized via USB ↔ RS232 FT232BM converter

⁴ Not available on Mod. N1470AL

⁵ RS 485 Serial Port Interface allows to control up to 32 modules connected by a twisted pair cable; the first and last modules must be terminated, see § 0.

2.5 Rear panel connections

2.5.1 HV Channel Output

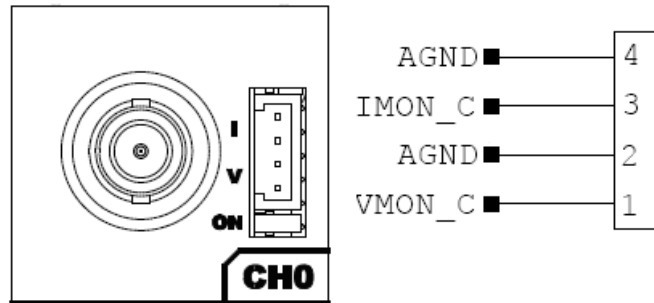


Fig. 2.11: HV Channel panel and test point electrical scheme

NAME:	TYPE:	FUNCTION:
MON	AMP 280371-2	Vout/Iout Test point
OUT	SHV RADIAL R317580	HV Channel Output
	Impedance: 50 Ohm	
	Frequency range: 0 – 2 GHz	
	VSWR: <1.20 + 0.3 F (GHz) – (plug and jack)	
	Test voltage: 10kV DC – 1mn (unmated connectors)	
	12kV DC – 1mn (mated pairs)	
	Current rating: 10 A	
ON	Red LED	HV Channel ON

The test points allow to monitor the Channel Output Voltage and Current according to the following conversion:

VMON: Voltage level (1V = 1.8kV $\pm$ 1% readout; same polarity as channel)

IMON high range: Voltage level (1V = 660 μ A $\pm$ 3% readout; positive, 0÷5 V range)

IMON low range: Voltage level (1V = 66 μ A $\pm$ 3% readout; positive, 0÷5 V range)



WARNING! These connectors produce extremely hazardous high voltages at a potentially lethal current level; never connect or disconnect the HV OUT connector with the crate power ON/OFF switch ON; always switch crate power OFF and wait at least 30s before connecting or disconnecting HV cables.

2.6 Imon Zoom

Imon Zoom allows to monitor the channel current with an increased resolution (10x) in the 0 – 300 μ A range; by selecting Imon Range = LOW (see § 3.2.2), the output current is monitored with 5nA resolution (instead of 50 nA), in the 0 – 300 μ A range. It is important to notice that, if Imon Range = LOW is selected, and the channel draws a current larger than 300 μ A, then Overcurrent is signalled.

2.7 Technical specifications table

Table 2.3: Mod. N1470 series channel technical specifications

Packaging			Single width NIM unit		
Output channels:			4 / 2 / 1 channels, Common Floating Return, SHV connector. Positive or Negative Polarity (requires internal setting, see § 4.1)		
Output ranges:			If IMON RANGE = High: 8 kV / 3 mA If IMON RANGE = Low ⁶ : 8 kV / 300 µA		
Max. Ch. Output Power:			9 W (Vset ≤ 3 kV) 8 W (Vset > 3 kV)		
Vset / Vmon Resolution:			200 mV		
Iset Resolution			50 nA		
Imon Resolution:			If IMON RANGE = High is selected resolution is 50 nA If IMON RANGE = Low ⁶ is selected resolution is 5 nA		
Vmax:			0 ÷ 8100 V Absolute maximum HV level that the channel is allowed to reach, independently from the preset value Vset. Output voltage cannot exceed the preset value Vmax. The accuracy is 1 % ± 5 V		
Vmax resolution:			± 1 V		
Alarm output:			Open collector, 100 mA maximum sink current		
Interlock input:			LOW: <1V; current~5mA; HIGH: 4÷6 V		
Ramp Up/Down:			1÷500 Volt/s, 1 Volt/s step		
Trip:			Max. time an "overcurrent" is allowed to last (seconds). A channel in "overcurrent" works as a current generator; output voltage varies in order to keep the output current lower than the programmed value. "Overcurrent" lasting more than set value (1 to 9999) causes the channel to "trip". Output voltage will drop to zero either at the Ramp-down rate or at the fastest available rate, depending on Power Down setting; in both cases the channel is put in the OFF state. If trip= INFINITE, "overcurrent" lasts indefinitely. TRIP range: 0 ÷ 999.9 s; 1000 s = Infinite. Step = 0.1 s		
Accuracy: ⁷		Vmon vs. Vout	±0.02% of read value ±2V		
		Vset vs. Vmon	±0.02% of read value ±2V		
		Imon vs. Iout	If IMON RANGE = High: ±2% of read value ±2 µA If IMON RANGE = Low ⁶ : ±2% of read value ±200 nA		
		Iset vs. Iout	If IMON RANGE = High: ±2% of read value ±2 µA If IMON RANGE = Low ⁶ : ±2% of read value ±200 nA		
Voltage Ripple	Range		3kV/200µA	3kV/3mA	8kV/800µA
	20 ÷ 1000 Hz	Typical	20 mVpp	20 mVpp	25 mVpp
		Maximum	25 mVpp	30 mVpp	30 mVpp
	1 ÷ 20000 kHz	Typical	5 mVpp	5 mVpp	10 mVpp
		Maximum	10 mVpp	10 mVpp	15 mVpp
Humidity range:			0 ÷ 80%		
Operating temperature:			0 ÷ 45°C		
Storage temperature:			-10 ÷ 70°C		
Vout / Temperature coefficient:			max. 50ppm / °C		
Imon / Temperature coefficient:			max 100ppm/C°; max 300ppm/C° with Imon X10 zoom ⁸		
Long term stability Vout vs. Vset:			± 0.02% (after one week @ constant temperature)		

⁶ Imon Zoom active see § 2.6.

⁷ From 10% to 90% of Full Scale Range

⁸ Typical data for IMON X10: Imon-Zoom Offset = $\pm$ 100nA; ppm/C° Imon-Zoom <300ppm/C°; Imon leakage +5nA/2kV

3 Operating modes



CAUTION: N1470 MUST BE USED ONLY IN CRATES WITH FORCED COOLING AIR FLOW!

Module control can take place either locally, or remotely, via USB or RS485 (see § 3.4).

3.1 Safety requirements and Initial inspection

N.B. read carefully the “Precautions for Handling, Storage and Installation” document provided with the product before starting any operation!

The following HAZARD SYMBOLS are reported on the unit:



CAUTION: indicates the need to consult the “Precautions for Handling, Storage and Installation” document provided with the product. **A potential risk exists if the operating instructions are not followed**



HIGH VOLTAGE: indicates the presence of electric shock hazards. Enclosures marked with these symbols should only be opened by CAEN authorized personnel.

To avoid risk of injury from electric shock, do not open this enclosure

To avoid potential hazards, use the product only as specified. Only qualified personnel should perform service procedures.

Avoid Electric Overload. To avoid electric shock or fire hazard, do not power a load outside of its specified range.

Avoid Electric Shock. To avoid injury or loss of life, do not connect or disconnect cables while they are connected to a voltage source.

Do Not Operate without Covers. To avoid electric shock or fire hazard, do not operate this product with covers or panels removed.

Do Not Operate in Wet/Damp Conditions. To avoid electric shock, do not operate this product in wet or damp conditions.

Do Not Operate in an Explosive Atmosphere. To avoid injury or fire hazard, do not operate this product in an explosive atmosphere.

Do Not Operate with Suspected Failures. If you suspect this product to be damaged, have it inspected by qualified service personnel.


3.2 Programmable parameters

3.2.1 Boards parameters

General board parameters (CONTROL can be operated both in LOCAL and REMOTE mode; other monitor and settings are allowed in LOCAL mode only; see § 3.3.2) include:

Parameter:	Function:
Power (Monitor)	Module power supply status
Termination (Monitor)	Local Bus termination status (ON/OFF)
HV Clock (Monitor)	Sync clock frequency (200±10 kHz correct value)
Local Bus Baud Rate (Monitor/Set)	9600, 19200, 38400, 57600, 115200 Baud

Display:






Local Bus Address (Monitor/Set)	Local Bus address for remote communication (0÷31)
USB Baud Rate (Monitor/Set)	9600, 19200, 38400, 57600, 115200 Baud
INTERLOCK (Monitor/Set)	CLOSED / OPEN OPERATION (see § 2.4.3)
CONTROL (Monitor/Set)	REMOTE: the module is controlled remotely; local monitor is allowed; LOCAL/REMOTE switch is enabled LOCAL: the module is controlled locally; remote monitor is allowed



3.2.2 Channel settings

For each channel the following parameters can be programmed and monitored either locally or remotely (see § 3.3.3):

Parameter:	Function:	Unit:	Display:
Vmon	High Voltage Monitored value	Volt	
Imon	Current Monitored value	μ A	
Vset	High Voltage programmed value	Volt	
Iset	Current Limit programmed value	μ A	
MaxV	Absolute maximum High Voltage level that the channel is allowed to reach (see § 2.7)	V	
Ramp-Up	Maximum High Voltage increase rate	V/s	
Ramp-Down	Maximum High Voltage decrease rate	V/s	
Power Down	Power Down mode after channel TRIP	KILL or RAMP	
Trip	Maximum time an "overcurrent" is allowed to last expressed in seconds (see § 2.7)	s	
Imon Range	Current Monitor Zoom 10x	High or Low	

3.3 Local Control

Insert the unit inside a powered NIM crate, and switch it ON. At the power the Display shows for a few seconds the following screen.

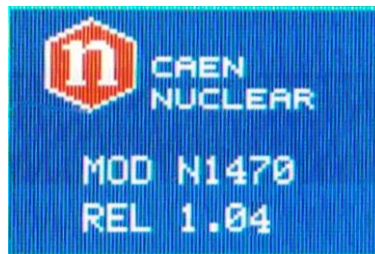


Fig. 3.1: Welcome screen

At this point the module is ready to be operated locally. The TUNE ROTARY SWITCH (see § 2.4.1) is lit up as long as Local Control is enabled.

3.3.1 HV connection

Verify the channels polarity (polarity setting is explained in § 3.5) checking that the polarity LEDs are switched on according to the programmed configuration (see § 2.4.2); verify the HV_EN/OFF/KILL 3 POS. SWITCH of each channel is set to OFF; the Display will show the following message in the left lower row:



Fig. 3.2: Channel OFF status screen

now connect the HV cable linking the outputs to the loads to be supplied and enable the HV outputs switching the HV_EN/OFF/KILL 3 POS. SWITCH in the HV_EN position; the Display will show the following message in the left lower row:

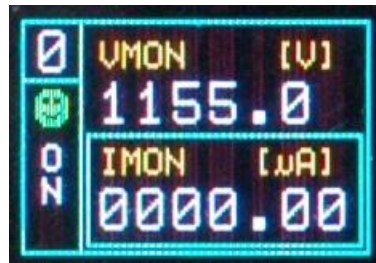


Fig. 3.3: Channel ON status screen

The KILL position of the HV_EN/OFF/KILL 3 POS. SWITCH allows to turn off the module at the fastest available rate; the Display will show the following message in the left lower row:

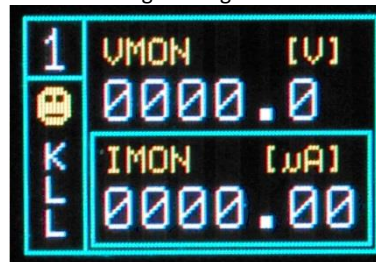


Fig. 3.4: Channel KILL status screen

3.3.2 Module settings

Module settings are general board settings; turn the TUNE ROTARY SWITCH until this screen is shown:

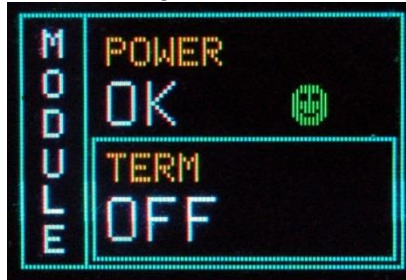


Fig. 3.5: Mode settings status screen

Push the TUNE ROTARY SWITCH in order to access MODULE parameters; the MODULE frame becomes red:

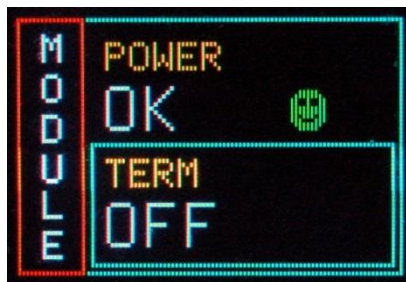


Fig. 3.6: Mode settings access screen

The TUNE ROTARY SWITCH allows to select the parameter to be set; turn the ROTARY SWITCH until such parameter is displayed (for example CONTROL), then select it by pushing the ROTARY SWITCH (the parameter is shown with a red frame as long as it is active):



Fig. 3.7: Mode settings edit screen

Select the desired value by turning the TUNE ROTARY SWITCH and confirm it by pushing the switch itself.

3.3.3 Channel settings

In order to operate Output Channel settings:

Turn the TUNE ROTARY SWITCH until the channel number to be set is displayed in the left upper row (for example Channel 0)

Push the TUNE ROTARY SWITCH: at this point the frame of the left upper row (channel number) becomes red and the channel is selected



Fig. 3.8: Channel settings edit screen

Turn the TUNE ROTARY SWITCH until the parameter to be set (for example VSET) is displayed in the right lower row



Fig. 3.9: Channel VSET select screen

Push the TUNE ROTARY SWITCH: at this point the parameter is selected, its frame is shown in red and its name in blue; it is now possible to change the parameters value



Fig. 3.10: Channel VSET access screen

Turn the TUNE ROTARY SWITCH until the value digit to be edited is shown in blue, the parameter name in yellow



Fig. 3.11: Channel VSET digit selection screen

Push the TUNE ROTARY SWITCH: at this point the value digit becomes yellow and can be edited



Fig. 3.12: Channel VSET digit access screen

Turn the TUNE ROTARY SWITCH until the digit reaches the desired value



Fig. 3.13: Channel VSET digit adjust screen

Confirm it by pushing the TUNE ROTARY SWITCH, the edited digit returns blue



Fig. 3.14: Channel VSET digit confirm screen

Once all the digits are set to the desired value, turn the TUNE ROTARY SWITCH until the parameter name returns blue



Fig. 3.15: Channel VSET confirm screen

Push the TUNE ROTARY SWITCH in order to de-select the parameter, the frame returns to blue



Fig. 3.16: Channel VSET de-select screen

It is now possible to set another parameter; note that the POWER DOWN and IMRANGE setting has not digits to be edited, but two options, TRIP/KILL and HIGH/LOW respectively:



Fig. 3.17: Channel KILL screen

In order to access another channel, the EXIT parameter has to be selected



Fig. 3.18: Channel EXIT screen

Now by turning the TUNE ROTARY SWITCH another channel number to be set can be selected.

If CONTROL MODE (see § 3.2.1) is set to REMOTE, the left lower row reports DIS (Disabled), since the channel can be accessed only via the serial links (see § 3.4.1). If the INTERLOCK MODE is changed while one channel is ON, the channel is turned OFF and the left lower row reports ILK (Interlock); if the channel is OFF, it can not be turned ON, until it is enabled according to the Interlock logic (see § 3.2.1).

3.3.3.1 Group Settings⁹

Group settings allow to broadcast the same parameter value to all channels.

In order to operate Group settings:

Turn the TUNE ROTARY SWITCH until ALL is displayed in the left column



Fig. 3.19: Group selection

Push the TUNE ROTARY SWITCH: at this point the frame of the left column becomes red and the GROUP is selected. Turn the TUNE ROTARY SWITCH until the parameter to be set (for example VSET) is displayed in the right column (all four channels values).

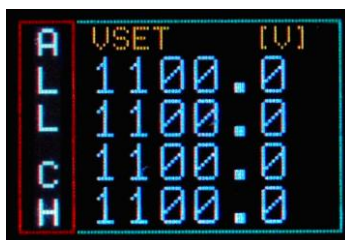


Fig. 3.20: Group active

Push the TUNE ROTARY SWITCH: at this point the parameter is selected, its frame is shown in red and its name in blue (only one value common to all channels; pre-set value is picked from Channel 0); it is now possible to change the parameters value.



Fig. 3.21: Group VSET access screen

Turn the TUNE ROTARY SWITCH until the value digit to be edited is shown in yellow, the parameter name in yellow



Fig. 3.22: Group VSET digit selection screen

Push the TUNE ROTARY SWITCH: at this point the value digit becomes yellow and can be edited

⁹ Mod. N1470B has not group settings; Mod. N1470A has group settings, 2 channels values are displayed



Fig. 3.23: Group Channel VSET digit access screen

Turn the TUNE ROTARY SWITCH until the digit reaches the desired value



Fig. 3.24: Group VSET digit adjust screen

Confirm it by pushing the TUNE ROTARY SWITCH, the edited digit returns blue



Fig. 3.25: Group VSET digit confirm screen

Once all the digits are set to the desired value, turn the TUNE ROTARY SWITCH until the parameter name returns blue. Push the TUNE ROTARY SWITCH in order to de-select the parameter, the frame returns to blue; when the parameter is not active, the parameter status of the four channels is shown.



Fig. 3.26: Channel VSET de-select screen

In order to go to individual channel settings, the EXIT parameter has to be selected



Fig. 3.27: Group EXIT screen

3.3.3.2 Smileys

Three types of Smileys in the display indicate:

Table 3.1: Smileys list

Smiley	Meaning
	OK Status
	WARNING Status
	ALARM Status

3.4 Remote Control

Module control can take place remotely, via USB or RS485; the latter allows to build a N1470s' daisy chain network. The CAEN NIM8301 7U 12 Slot Smart Fan Unit 300/600 W Crate allows also to communicate with the module via Ethernet.

3.4.1 Serial Links

3.4.1.1 USB communication

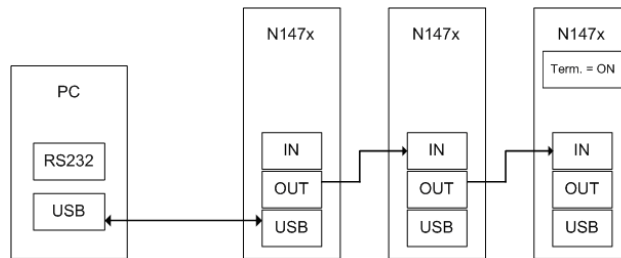


Fig. 3.28: USB communication diagram

The module is provided with a USB2.0 compliant interface (see § 2.4.4). The N1470 can be programmed via PC by connecting the PC USB port with the N1470 USB B-type port; the featured controller, the FT232BM chip requires drivers freely available at www.ftdichip.com (Drivers section); the site also provides installation instructions for all OS's (Documents section)

The connection can be performed via terminal emulator, such as HyperTerminal, configured as follows:

- baud rate 9600 (the same set on the N1470! See § 3.3.2)
- Data bits: 8
- Parity: none
- stop bit: 1
- Flow control: Xon Xoff

It is also possible to build a daisy chain of up to 32 N1470's, with the first module connected to the PC USB port and the subsequent ones daisy chained through the COMM IN/OUT, as explained in § 3.4.1.3; in this case communication with the chained modules is achieved through the USB - RS485 Communication Protocol, see § 3.5. All modules must be assigned a LOCAL BUS ADDRESS (see § 3.2.1) different from one another and the last one must be terminated (see § 4.2.1).

3.4.1.4 Ethernet communication

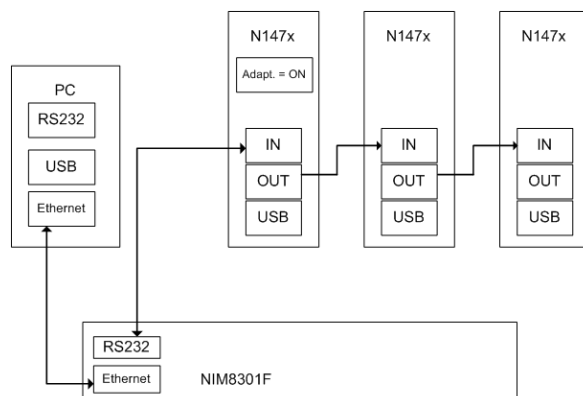


Fig. 3.31: Ethernet communication diagram

It is possible to communicate via Ethernet with one or more daisy chained N1470 modules through the NIM8301 Fan Unit¹⁰. Communication via Ethernet is possible only through the USB - RS485 Communication Protocol. The single module or the first module of the daisy chain must be connected to the Fan Unit RS232 port through the cable adapter (see figure below) connected to the N1470 COMM IN port; SW[200, 201] switch placed on the Microcontroller board inside the module must be set to Adaptation ON (see § 4.2.2).

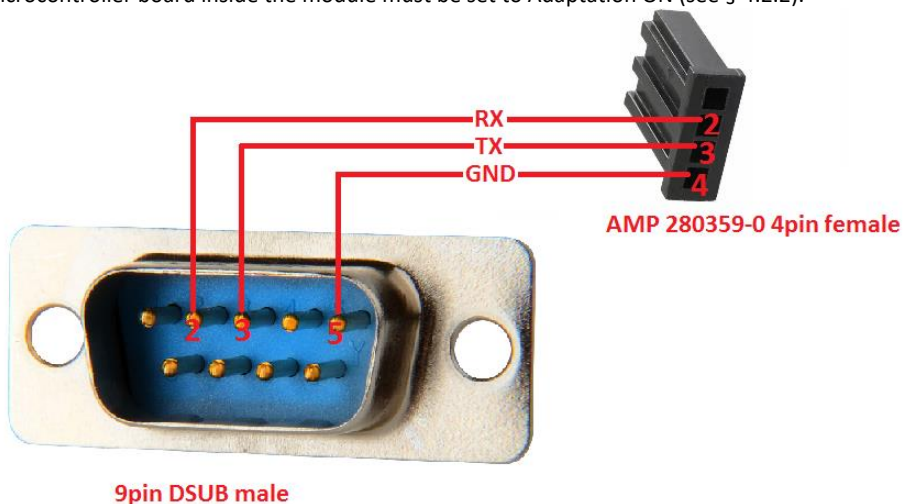


Fig. 3.32: RS232 port cable adapter

¹⁰ The CAEN Mod. NIM8301 is a 7U (5+2) full size NIM crate (19"-12 slot) available with pluggable 300W and 600W power supplies, ventilated by pluggable 2U fan unit. Remote control and monitoring take place through CAN bus, Ethernet, USB and RS232 interfaces.

3.4.2 Communication Control

In order to launch the communication, type **CAEN** and then <Enter>.
As the communication is established, the Main Menu will be displayed.

3.4.2.1 Remote Control: Main Menu

```

  ##  ##  ##  #####  #####  #####
  ###  ##  ####  ##  ##  ##  ##
  ##  ##  ##  #####  ##  ##  ##
  ##  ##  ##  ##  ##  ##  ##
  ##  ##  ####  #####  ##  #####

C.A.E.N. N1470 4 CH 8KV 3mA V1.00 Addr 08

B O A R D   M E N U

Display          Display/Modify channels
Format           Reformat EEPROM
General          General board status
Update           Firmware Update

Quit             Abandon program

Select Item
  
```

Fig. 3.33: Main Menu

Type **D** to set/monitor channels parameters
Type **F** to format the EEPROM
Type **G** to monitor board status
Type **U** to upgrade the firmware
Type **O** to perform the current offset calibration
Type **Q** to exit the program

3.4.2.2 Remote Control: General Menu

By typing **G** it is possible to access the General Menu which includes the board's general settings.

```

C.A.E.N. N1470 4 Ch HV Power Supply V1.00 Addr 00

Serial Number      : 35
Boot firmware Version : 1.0
Local Bus Termination : OFF
Interlock Active    : CLOSED
Internal Supply      : OK
Over Power           : NO
HV Clock [200 KHz]   : 199 KHz

Press 'I' to change Interlock Mode or any key to quit.
  
```

Fig. 3.34: Board Status Menu

3.4.2.3 Remote Control: Channels Menu

By typing **D** it is possible to monitor and set all the channels parameters listed in § 3.2.2

C.A.E.N. N1470 4 CH 8KV 3mA	V1.00	Addr 08	
	Ch0	Ch1	Ch2
Polarity	+	+	+
Vmon	0000.0 V	0000.0 V	0000.0 V
Imon	0000.00 mA	0000.00 uA	0000.00 uA
Status			
Power	Off	Off	Off
Vset	1000.0 V	2005.0 V	4000.0 V
Iset	2751.55 uA	0997.00 uA	1000.00 uA
Maxv	8100 V	8100 V	8100 V
Ramp Up	500 V/S	500 V/S	500 V/S
Ramp Down	500 V/S	500 V/S	500 V/S
Trip	Inf. S	Inf. S	Inf. S
Power Down	Kill	Kill	Kill
Group Mode	Reset Alarm	Quit	

Fig. 3.35: Channels Menu

In order to change one parameter: point the parameter with the arrow keys (see figure below), and type the desired value, confirm by pressing <Enter>; Power and Power Down can be changed using the <Space> bar.

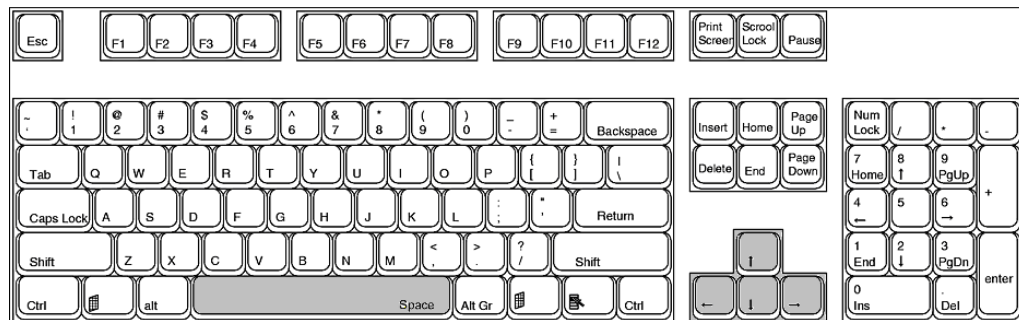


Fig. 3.36: PC keyboard

When one parameter is active, by typing G it is possible to make a “group setting”, i.e. broadcast the same value to all channels (the parameter becomes active on all channels, see figure).

C.A.E.N. N1470 4 Ch HV Power Supply	V1.00	Addr 00	
	Ch0	Ch1	Ch2
Polarity	+	+	+
Vmon	0000.0 V	0000.0 V	0000.0 V
Imon	0000.00 uA	0000.00 uA	0000.00 uA
Status	Dis	Dis	Dis
Power	Off	Off	Off
Vset	1100.0 V	1100.0 V	1100.0 V
Iset	3000.00 uA	3000.00 uA	3000.00 uA
Maxv	8100 V	8100 V	8100 V
Ramp Up	500 V/S	500 V/S	500 V/S
Ramp Down	500 V/S	500 V/S	500 V/S
Trip	Inf. S	Inf. S	Inf. S
Power Down	Kill	Kill	Kill
Imon Range	High	High	High
Group Mode	Reset Alarm	Quit	

Fig. 3.37: Channels group setting

Type Q to exit the Menu.

3.4.2.4 Remote Control: firmware upgrade

By typing U it is possible to access the firmware upgrade menu:

```
C.A.E.N. N1470 4 CH 8KV 3mA V1.00

Firmware Update. Are you sure ? [y/n] _
```

Fig. 3.38: Firmware Upgrade Menu/1

If <y> is typed, then the following menu is shown:

```
C.A.E.N. N1470 4 Ch HV Power Supply V1.00 Addr 00

Firmware Update. Are you sure ? [y/n]

When the message 'Firmware Updating Complete' is
displayed, wait few seconds and then press 'caen'.

Resetting ..
Flash Erasing ...
Ready to receive
Please send the new firmware
```

Fig. 3.39: Firmware Upgrade Menu/2

At this point it is necessary to upload the updated firmware.

If "HyperTerminal" is used it is necessary to perform "Transfer" and "Send Text File" operations by selecting the file "N1470.xxx"

3.4.2.5 Remote Control: format EEPROM

By typing F it is possible to access the format EEPROM menu:

```
C.A.E.N. N1470 4 CH 8KV 3mA V1.00

Format EEPROM. Are you sure ? [y/n]
```

Fig. 3.40: Format EEPROM Menu

After the FORMAT command, all the channels have the following settings:

Vset = 0 V
Iset = 300 μ A
Ramp Up / Down = 50 V/s
Trip = 10 s
MaxV = 8100 V
Power Down = Kill

Module setting:
Interlock Mode = Active CLOSED

3.5 USB - RS485 Communication Protocol

The following Protocol allows to communicate with up to 32 daisy chained modules. The Protocol is based on commands made of ASCII characters strings. The protocol requires firmware revision 1.0.1 or greater.

3.5.1 Command Format

The Format of a command string is the following :

\$BD:,CMD:***,CH*,PAR:***,VAL:***,**<CR, LF >**

The fields that form the command are :

BD : 0..31 module address (to send the command)

CMD : MON, SET

CH : 0..4 (4 for the commands related to all Channels)

PAR : (see parameters tables)

VAL : (numerical value must have a Format compatible with resolution and range)

3.5.2 Format of response string

Format response in case of error

String	Function (Units)
#BD:**,CMD:ERR	Wrong command Format or command not recognized
#BD:**,CH:ERR	Channel Field not present or wrong Channel value
#BD:**,PAR:ERR	Field parameter not present or parameter not recognized
#BD:**,VAL:ERR	Wrong set value (<Min or >Max)
#BD:**,LOC:ERR	Command SET with module in LOCAL mode

Each string is terminated by < **CR, LF** >

Format response in case of correct command

String	Function (Units)
#BD:**,CMD:OK	command Ok
#BD:**,CMD:OK,VAL:***	command Ok *** = value for command to individual Channel
#BD:**,CMD:OK,VAL:***,**	command Ok *** = values Ch0,1,2,3 for command to all Channels

Numerical value Field '**VAL**' has Format compatible (comma and decimal part) with the resolution and the range related to the parameter.

Each string is terminated by < **CR, LF** >

3.5.3 MONITOR commands related to the Channels

The following table contains the strings to be used to handle monitor commands related to the Channels.

The '**X**' in the Field 'Channel' can be set in the '**0..(N-1)**' range¹¹.

When '**X=N**' the module returns the values of the parameter of all N Channels.

String	Function (Units)
\$BD:xx,CMD:MON,CH:X,PAR:VSET	Read out VSET value (XXXX.X V)
\$BD:xx,CMD:MON,CH:X,PAR:VMIN	Read out VSET minimum value (0 V)
\$BD:xx,CMD:MON,CH:X,PAR:VMAX	Read out VSET maximum value (8000.0 V)
\$BD:xx,CMD:MON,CH:X,PAR:VDEC	Read out VSET number of decimal digits
\$BD:xx,CMD:MON,CH:X,PAR:VMON	Read out VMON value (XXXX.X V)
\$BD:xx,CMD:MON,CH:X,PAR:ISET	Read out ISET value (XXXX.XX μ A)
\$BD:xx,CMD:MON,CH:X,PAR:IMIN	Read out ISET minimum value (0 μ A)
\$BD:xx,CMD:MON,CH:X,PAR:IMAX	Read out ISET maximum value (3000.00 μ A)
\$BD:xx,CMD:MON,CH:X,PAR:ISDEC	Read out ISET number of decimal digits
\$BD:xx,CMD:MON,CH:X,PAR:IMON	Read out IMON value (XXXX.XX μ A)
\$BD:xx,CMD:MON,CH:X,PAR:IMRANGE	Read out IMON RANGE value (HIGH / LOW)
\$BD:xx,CMD:MON,CH:X,PAR:IMDEC	Read out IMON number of decimal digits (2 HR, 3 LR)
\$BD:xx,CMD:MON,CH:X,PAR:MAXV	Read out MAXVSET value (XXXX V)
\$BD:xx,CMD:MON,CH:X,PAR:MVMIN	Read out MAXVSET minimum value (0 V)
\$BD:xx,CMD:MON,CH:X,PAR:MVMAX	Read out MAXVSET maximum value (8100 V)
\$BD:xx,CMD:MON,CH:X,PAR:MVDEC	Read out MAXVSET number of decimal digits

¹¹ **N** is the number of channels

String	Function (Units)
\$BD:xx,CMD:MON,CH:X,PAR:RUP	Read out RAMP UP value (XXX V/S)
\$BD:xx,CMD:MON,CH:X,PAR:RUPMIN	Read out RAMP UP minimum value (1 V/S)
\$BD:xx,CMD:MON,CH:X,PAR:RUPMAX	Read out RAMP UP maximum value (500 V/S)
\$BD:xx,CMD:MON,CH:X,PAR:RUPDEC	Read out RAMP UP number of decimal digits
\$BD:xx,CMD:MON,CH:X,PAR:RDW	Read out RAMP DOWN value (XXX V/S)
\$BD:xx,CMD:MON,CH:X,PAR:RDWMIN	Read out RAMP DOWN minimum value (1 V/S)
\$BD:xx,CMD:MON,CH:X,PAR:RDWMAX	Read out RAMP DOWN maximum value (500 V/S)
\$BD:xx,CMD:MON,CH:X,PAR:RDWDEC	Read out RAMP DOWN number of decimal digits
\$BD:xx,CMD:MON,CH:X,PAR:TRIP	Read out TRIP time value (XXXX.X S)
\$BD:xx,CMD:MON,CH:X,PAR:TRIPMIN	Read out TRIP time minimum value (0 S)
\$BD:xx,CMD:MON,CH:X,PAR:TRIPMAX	Read out TRIP time maximum value (1000.0 S)
\$BD:xx,CMD:MON,CH:X,PAR:TRIPDEC	Read out TRIP time number of decimal digits
\$BD:xx,CMD:MON,CH:X,PAR:PDWN	Read out POWER DOWN value (RAMP / KILL)
\$BD:xx,CMD:MON,CH:X,PAR:POL	Read out POLARITY value ('+' / '-')
\$BD:xx,CMD:MON,CH:X,PAR:STAT	Read out Channel status value (XXXXX)

3.5.3.1 Meaning of STATUS bits (value read in decimal Format)

Bit	Function
Bit 0 → ON	1 : ON 0 : OFF
Bit 1 → RUP	1 : Channel Ramp UP
Bit 2 → RDW	1 : Channel Ramp DOWN
Bit 3 → OVC	1 : IMON >= ISET
Bit 4 → OVV	1 : VMON > VSET + 250 V
Bit 5 → UNV	1 : VMON < VSET - 250 V
Bit 6 → MAXV	1 : VOUT in MAXV protection
Bit 7 → TRIP	1 : Ch OFF via TRIP (Imon >= Iset during TRIP)
Bit 8 → OVP	1 : Power Max Power Out > 9.3W for VOUT ≤ 3KV Power Out > 8.2W for VOUT > 3KV
Bit 9 → OVT	1: TEMP > 105°C
Bit 10 → DIS	1 : Ch disabled (REMOTE Mode and Switch on OFF position)
Bit 11 → KILL	1 : Ch in KILL via front panel
Bit 12 → ILK	1 : Ch in INTERLOCK via front panel
Bit 13 → NOCAL	1 : Calibration Error
Bit 14, 15 → N.C.	

3.5.4 MONITOR commands related to the module

The following table shows the strings to be used to handle monitor commands related to the module.

String	Function (Units)
\$BD:xx,CMD:MON,PAR:BDNAME	Read out module name (N1470...)
\$BD:xx,CMD:MON,PAR:BDNCH	Read out number of Channels present (4, 2, 1)
\$BD:xx,CMD:MON,PAR:BDFREL	Read out Firmware Release (XX.X)
\$BD:xx,CMD:MON,PAR:BDSNUM	Read out value serial number (XXXXX)
\$BD:xx,CMD:MON,PAR:BDILK	Read out INTERLOCK status (YES/NO)
\$BD:xx,CMD:MON,PAR:BDILKM	Read out INTERLOCK mode (OPEN/CLOSED)

String	Function (Units)
\$BD:xx,CMD:MON,PAR:BDCTR	Read out Control Mode (LOCAL / REMOTE)
\$BD:xx,CMD:MON,PAR:BDTERM	Read out LOCAL BUS Termination status (ON/OFF)
\$BD:xx,CMD:MON,PAR:BDALARM	Read out Board Alarm status value (XXXXX)

3.5.4.1 Meaning of Board Alarm bits

Bit	Function
Bit 0 → CH0	1 : Ch0 in Alarm status
Bit 1 → CH1	1 : Ch1 in Alarm status
Bit 2 → CH2	1 : Ch2 in Alarm status
Bit 3 → CH3	1 : Ch3 in Alarm status
Bit 4 → PWFAIL	1 : Board in POWER FAIL
Bit 5 → OVP	1 : Board in OVER POWER
Bit 6 → HVCKFAIL	1 : Internal HV Clock FAIL (≠ 200±10kHz)

3.5.5 SET commands related to the Channels

The following table contains the strings to be used to handle set commands related to the Channels.
The 'X' in the Field 'Channel' can be set to the '0..(N-1)' values.
When 'X=N' the command is issued to all N Channels.

String	Function (Units)
\$BD:xx,CMD:SET,CH:X,PAR:VSET,VAL:XXXX.X	Set VSET value
\$BD:xx,CMD:SET,CH:X,PAR:ISET,VAL:XXXX.XX	Set ISET value
\$BD:xx,CMD:SET,CH:X,PAR:MAXV,VAL:XXXX	Set MAXVSET value
\$BD:xx,CMD:SET,CH:X,PAR:RUP,VAL:XXX	Set RAMP UP value
\$BD:xx,CMD:SET,CH:X,PAR:RDW,VAL:XXX	Set RAMP DOWN value
\$BD:xx,CMD:SET,CH:X,PAR:TRIP,VAL:XXXX.X	Set TRIP time value
\$BD:xx,CMD:SET,CH:X,PAR:PDWN,VAL:RAMP/KILL	Set POWER DOWN mode value
\$BD:xx,CMD:SET,CH:X,PAR:IMRANGE,VAL:HIGH/LOW	Set IMON RANGE value
\$BD:xx,CMD:SET,CH:X,PAR:ON	Set Ch ON
\$BD:xx,CMD:SET,CH:X,PAR:OFF	Set Ch OFF

3.5.6 SET commands related to the module

String	Function (Units)
\$BD:xx,CMD:SET,PAR:BDILKM,VAL:OPEN/CLOSED	Set Interlock Mode
\$BD:xx,CMD:SET,PAR:BDCLR	Clear alarm signal

4 Internal Settings

4.1 Polarity selection

The output polarity is independently selectable for each channel. Note that the polarity is indicated by two LEDs for each channel on the front panel.

In order to change the polarity:

- Wear Antistatic Gloves
- Switch off the unit
- Wait for the complete discharge of the capacitors.
- Lay down the unit, right side up
- Remove screws 1, 2, 3, 4, 5, 6, see figure (red):

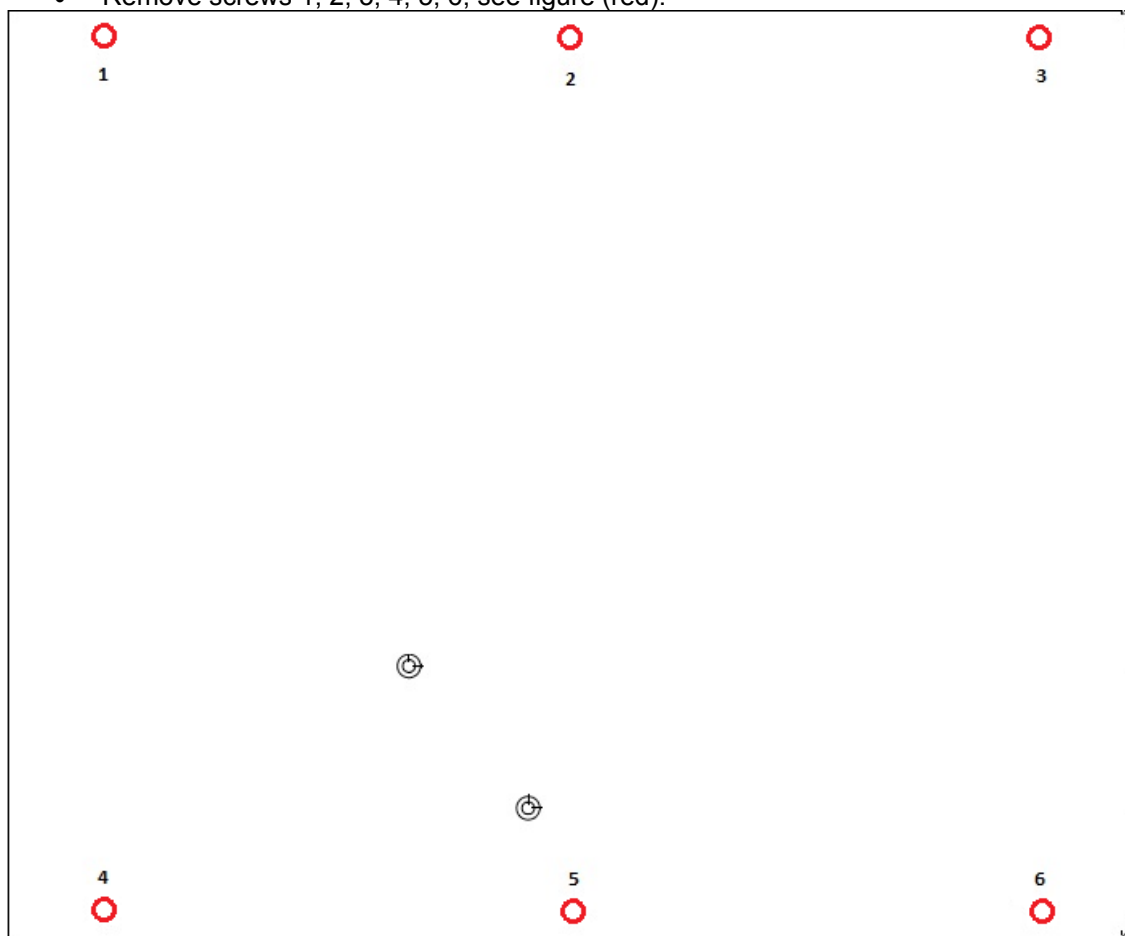


Fig. 4.1: Side cover removal instructions

- Lift the side cover gently
- At this point it is possible to change the channel polarity: refer to the following figure (the blue arrow indicates diode bridge box placed to configure channel as POSITIVE).
- During this operation pay attention not to bend the pins, as they are plugged completely in their sockets

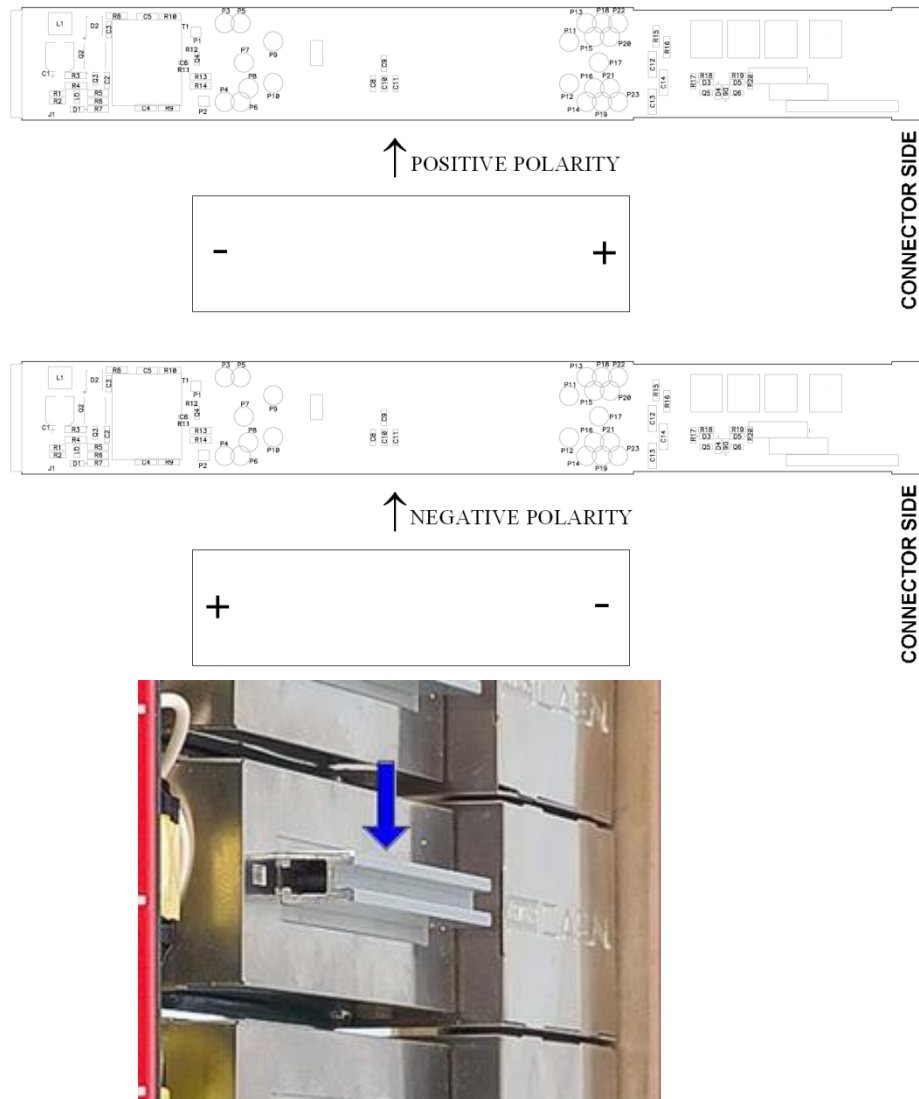


Fig. 4.2: Polarity selection instructions

- In order to choose the POSITIVE POLARITY, plug the diode bridge box, with the + symbol towards the connector side.
- In order to choose the NEGATIVE POLARITY, plug the diode bridge box, with the - symbol towards the connector side.
- Always pull and plug the diode bridge box by holding it on the handle pointed by the arrow in Fig. above.
- Once settings are done, put the right side cover back in place with screws 1, 2, 3, 4, 5, 6.

4.2 Internal switches

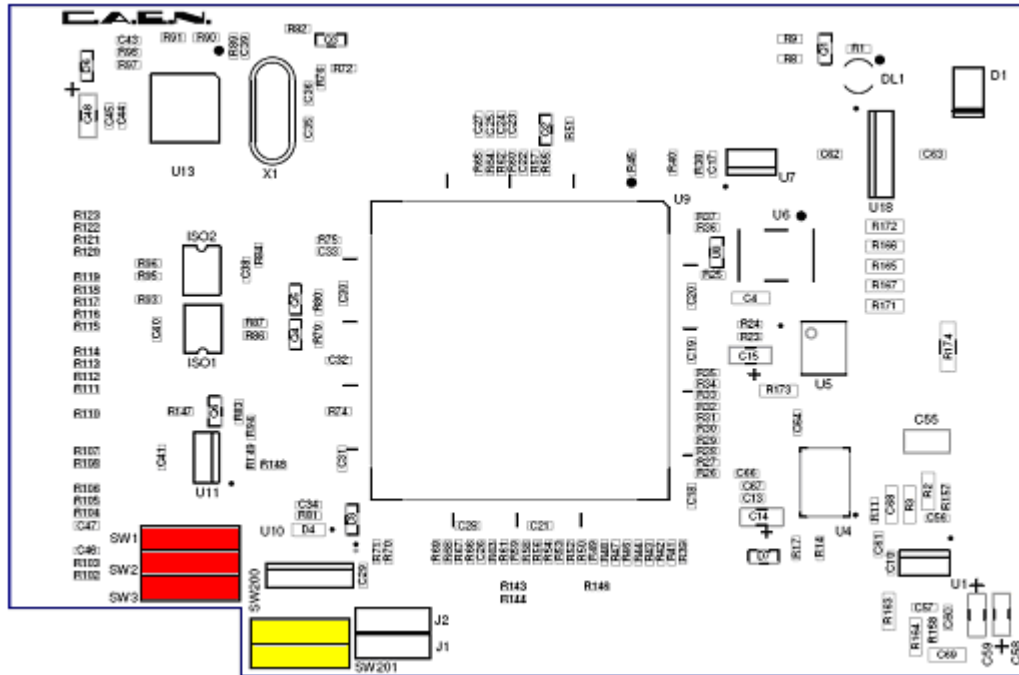


Fig. 4.3: Dip switch position

4.2.1 Local Bus termination

The SW[1..3] switch placed on the Microcontroller board inside the module (behind the *Remote communication control* section, see § 2.4.4), allows to terminate the Local Bus for daisy chain purposes (see § 3.4.1); dot NOT visible = Termination ON.

4.2.2 RS485 – RS232 conversion

The SW[200, 201] switch placed on the Microcontroller board inside the module, allows to adapt RS485 signals to RS232; dot visible = Adaptation ON.

4.3 Grounding specifications

The Mod. N14xx channels share a common floating return (FAGND), insulated from the crate ground (AGND). This feature allows on-detector grounding, thus avoiding loops which may increase noise level. FAGND and AGND may be connected, by short circuiting C21 jumper pins on the motherboard (see figure below). The protection shield must be screwed off in order to access C21 (see 4.1).

Please note that older versions of the N14xx may not have C21 jumper installed; contact info@caen.it for details.

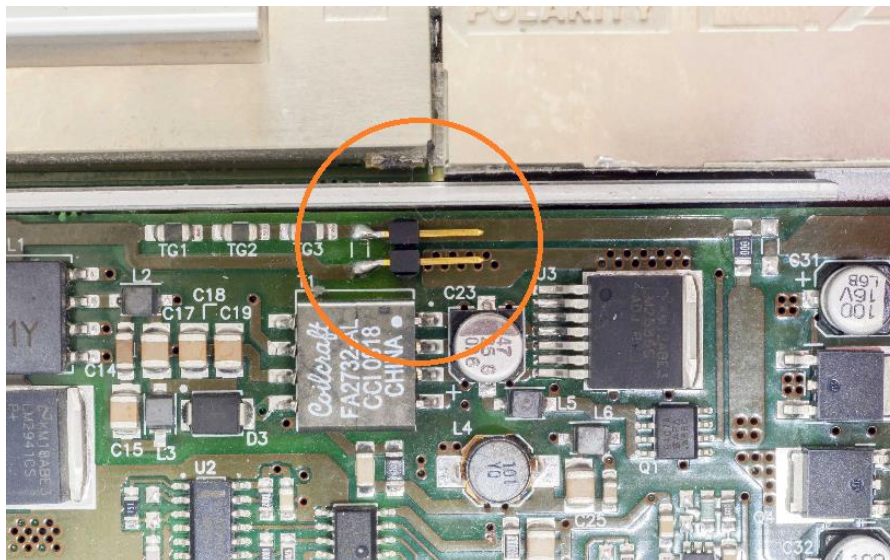


Fig. 4.4: C21 jumper location

4.3.1 Safety Earth connection

The connection of return to Earth is fundamental for User safety. The connection must always be at the level of detector or power supply system.

Return connection even if not present or performed incorrectly, due to protection circuits implemented on the N14xx are bound to Earth; in this case the voltage difference between return and Earth (System), is limited to approximately 50V. Please note that this is a status of emergency-protection, not a working one. The Connector Configurator allows to optimize the connection of the return and of AGND (Earth). The best configuration must be determined by the user upon application, the optimal connection depends on many characteristics of the related experiment.

The following diagrams show two examples of configuration, namely:

The "closed loop " Earth configuration (C21 contacts closed)

The "open loop" Earth configuration (C21 contacts open)

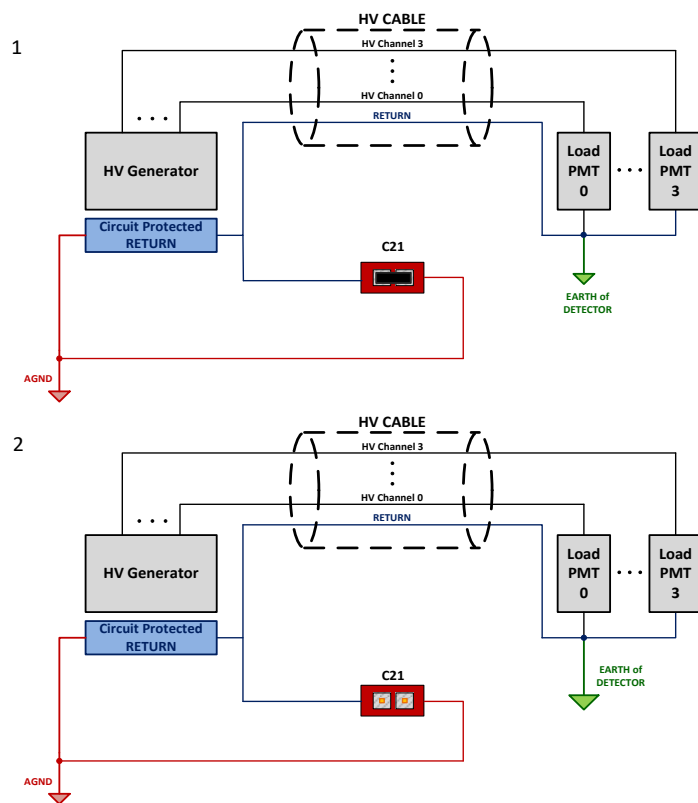
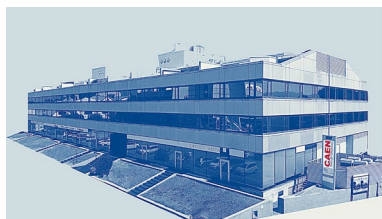


Fig. 4.5: Earth configuration connection examples

**CAEN S.p.A.**

Via Vetraria 11
55049 - Viareggio
Italy
Phone +39 0584 388 398
Fax +39 0584 388 959
info@caen.it
www.caen.it

**CAEN GmbH**

Brunnenweg 9
64331 Weiterstadt
Germany
Tel. +49 (0)212 254 4077
Mobile +49 (0)151 16 548 484
info@caen-de.com
www.caen-de.com

CAEN Technologies, Inc.

1 Edgewater Street - Suite 101
Staten Island, NY 10305
USA
Phone: +1 (718) 981-0401
Fax: +1 (718) 556-9185
info@caentechnologies.com
www.caentechnologies.com

CAENspa INDIA Private Limited

B205, BLDG42, B Wing,
Azad Nagar Sangam CHS,
Mhada Layout, Azad Nagar, Andheri (W)
Mumbai, Mumbai City,
Maharashtra, India, 400053
info@caen-india.in
www.caen-india.in



Copyright © CAEN SpA. All rights reserved. Information in this publication supersedes all earlier versions. Specifications subject to change without notice.